


MODALIZER+

User's Manual

Version 6.1

HEALTHCARE IMAGING WORKFLOW WIZARD

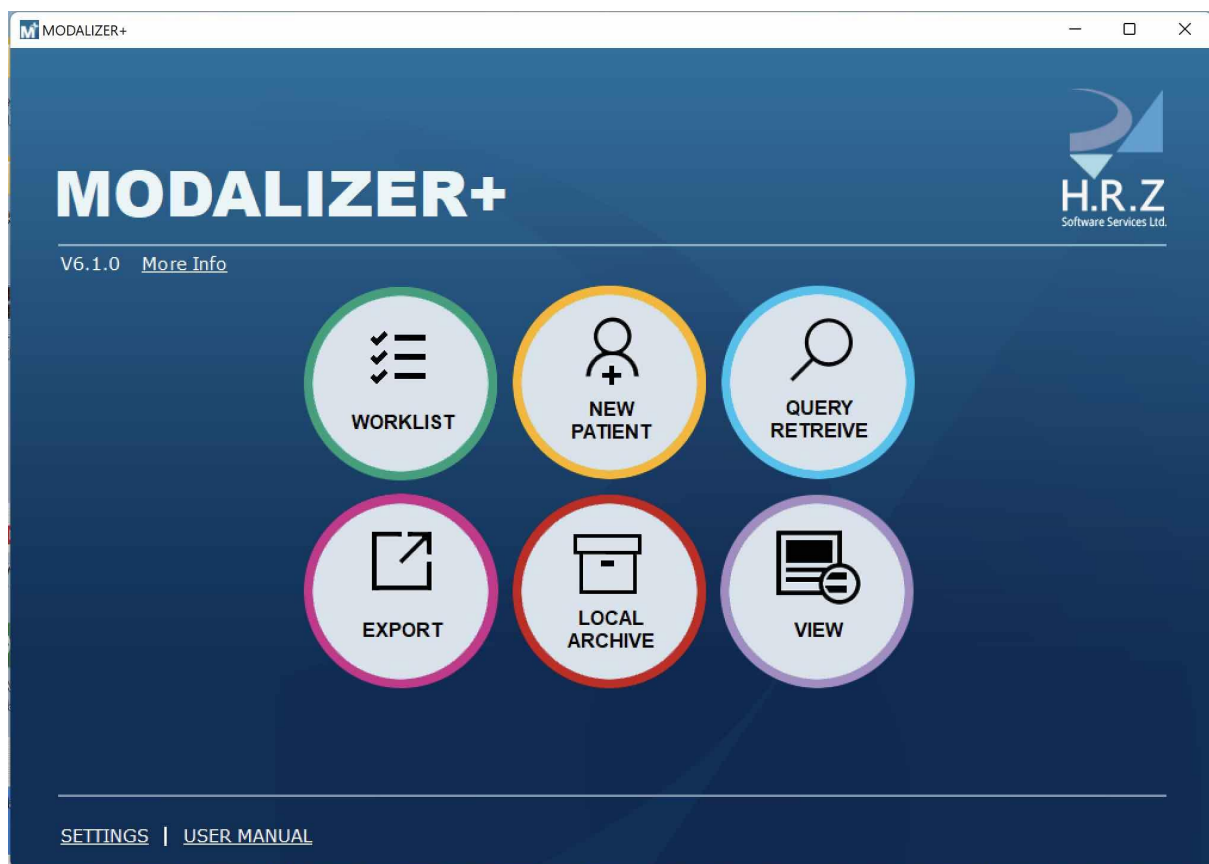

H.R.Z Software Services LTD

www.hrzkkit.com

info@hrzkkit.com





Reference Documents

Title	Date	Link
DICOM Conformance Statement	March 6, 2023	MODALIZER+ V6.1 DICOM CONFORMANCE STATEMENT.pdf



Table of Contents

Reference Documents	2
1. Introduction	4
1.1. Why convert to DICOM?	5
1.2. Supported Image and Document Types	5
1.3. Free DICOM viewer	6
2. Quick Start	7
2.1. The New Patient Wizard (Yellow)	7
2.2. Capturing Images and Scanning Documents	7
2.3. Filling a Report	11
2.4. Export DICOM Removable Media (CD/DVD/USB)	11
2.5. Viewing DICOM files	12
2.6. Connecting To PACS	12
2.7. The Local Archive	12
3. DICOM Viewer	13
3.1. Loading images to the Viewer	15
4.2. Using Hounsfield units Contrast Presets	21
4.3. Distance /Optical Density / Angle Measurements tools	23
4.4. ECG Viewer	29
4.5. Using Zoom/Pan/Contrast/Scroll tools	29
4.6. Flip and Rotate tool	30
4.7. CINE tool	32
4.8. Display Grayscale Softcopy Presentation State module	33
4.9. The DICOM Header view (editing DICOM objects)	34
5. Working with Studies	39
5.2. New Patient	39
5.3. Sending DICOM Images to the PACS	42
5.4. Modality Worklist Query	44
5.5. Query/Retrieve - Searching the PACS	46
5.6. Export - Burn CD/DVD	47
6. Reporting	49
6.2. Formatted Report Templates	49
6.3. DICOM Structured Reports (DICOM SR)	50
7. The Local Archive	51
8. MODALIZER+ Settings	54
8.2. TLS (Transport Layer Security) Secure DICOM Networking	56
8.3. DICOM Listener configuration	56
8.4. Local Archive configuration	60
8.5. Storage Servers configuration	61



8.6. Worklist Servers configuration	63
8.7. External Acquisition Application configuration	65
8.8. Formatted Report Template configuration	67
8.9. Custom Actions configurations	68
8.10. DICOM templates - Override DICOM Attributes	70
8.11. ECG Display Settings	71
8.12. Misc configuration	71
8.12.1. File System Directory Organizations	71
8.12.2. Support of the Unicode character set	71
8.12.3. Per-User Configuration	71
8.12.4. Capture Key	72
8.12.5. DICOM Log level for operations as "Send ECHO", "Get Query" etc.	72
9. Completing tasks with MODALIZER+	73
9.2. Viewing DICOM Images	73
9.3. Using CD/DVD DICOM Viewer	73
9.4. Viewing PDF file in DICOM format	73
9.5. Attaching scanned documents to the patient folder	73
9.6. Sending the same study to multiple destinations	73
9.7. MPPS (Modality Performed Procedure Step)	74
10. Troubleshooting	74
10.2. Log Files	74
11. Command line parameters	75

1. Introduction

MODALIZER+ is a powerful and easy-to-use Point-of-Care Imaging and Reporting tool. It was carefully designed to capture, scan and display Images and documents in PACS Environment. MODALIZER+ provides a complete solution for Healthcare personnel to document patient encounters, attach media to the patient folder in the PACS, and perform other related tasks. MODALIZER+ is a state of the art DICOM Application with rich feature set combining Imaging Modality, Reporting Tool, DICOM Viewer and Conversion Tool:

- Capture, scan and convert Images from image files, USB Cameras, paper and film scanners and other TWAIN/WIA Imaging Devices, MPEG, PDF, JPG, PNG, TIFF, J2K and Bitmaps.
- Fully Customizable, auto-complete, PDF Report Templates.
- Integrate with a PACS to store, search, retrieve and display Images and Reports.



- Workflow Integration using DICOM Modality Worklist and Modality Performed Procedure Step to obtain Patient and Procedure parameters, report procedure progress, eliminate typos and reduce QA efforts.
- Multi-Modality Image Display and PACS Workstation - creating, connecting, searching, retrieving and storing images and documents on the PACS. Creating DICOM Media, Burning CD/DVD and USB with integrated DICOM CD Viewer.
- Manage your own medical image archive using the built-in Local Archive database.
- DICOM Listener.
- Customizable DICOM instances structure and content.
- Configurable “Capture Key” to take images using the keyboard or dedicated hardware such as pedal or external capture button.

1.1. System requirements

Computer: Microsoft Windows compatible laptop/desktop/tablet or virtual machine

Display resolution: minimum 1024x768 pixels

Operating systems: Microsoft Windows 8, 8.1 and 10

.NET Framework: 4.5

Processor: minimum recommended speed – 1Ghz

Internal memory: recommended minimum 1GB

Storage: recommended minimum 40GB of hard disk/SSD

Network Protocol: Secure DICOM Networking (TLS) over TCP/IP

USB: optional for external imaging hardware supporting VIA TWAIN/WIA: optional for paper scanner integration. Use the scanner vendor TWAIN driver utility for configuration of the scanning profile parameters.

1.2. Why convert to DICOM?

Digital Imaging and Communications in Medicine (DICOM) is the standard for handling, storing, printing, and transmitting medical images. DICOM is the most widely deployed healthcare-imaging standard in the world. DICOM images can be exchanged between two entities that are capable of receiving image and patient data in DICOM format.

DICOM enables the integration of scanners, archives, workstations, printers, and network hardware from multiple manufacturers into a picture archive and communication system (PACS).



1.3. Supported Image and Document Types

MODALIZER+ supports the following conversions: PDF, JPEG, PNG, BMP, TIF, Jpeg 2000, MPEG-2, MPEG-4. MODALIZER+ can convert a series of images of the same type and size to Multi-Frame DICOM objects stored in a single file.

1.4. Free DICOM viewer

MODALIZER+ includes a free DICOM Viewer. Click "Free Viewer" or drag-and-drop DICOM file/folder onto the application window to open the viewer screen. When closing the free viewer, MODALIZER+ will open HRZ Website in your browser.



2. Quick Start

This section is a quick step by step demonstration of MODALIZER+ Capabilities.

NOTE 1: You can open the user manual in the external PDF viewer from any screen of the application by clicking on the “User Manual” button at the bottom left corner of the application window.

NOTE 2: MODALIZER+ can be started from command line with parameters. See detailed description in the Command Line Parameters section of this document.

NOTE 3: Every function in the menu has a unique **color code** that continues through the operation. The color from the main menu item follows in the next screens icons and top separator.

2.1. The New Patient Wizard (Yellow)

- Click “New Patient” in the main menu.
- Enter the patient’s data. Click the ellipses to the right of the patient last name text box to add middle initial, prefix and suffix. Click “Next”.
- MODALIZER+ recognizes TWAIN/WIA Imaging Devices connected to your computer. You can select one of them using the drop-down menu on the top left corner of the image preview panel.
- Select files from your computer by clicking “Add files”. If the camera preview panel is visible, capture images by clicking the red button or [capture key](#) (if configured). You can also drag-and-drop files from your computer to the MODALIZER+ window. Click “Next”.
- To record video click the two circles red button that opens the video capture application.
- Select “Convert” for Action and then click “Next”.
- Click “Open destination folder”. The case folder where the converted file are stored will open.
- Click the “Done” button to return to the main menu.

For more details see [New Patient](#).

2.2. Capturing Images and Scanning Documents


MODALIZER+ Automatically detects and connects to TWAIN/WIA supporting devices such as the internal web camera of your laptop, USB cameras and most document Scanners. When a supported imaging device is detected, the capture and preview panels are automatically displayed. MODALIZER+ can work with multiple image sources simultaneously and can easily switch between devices within the same procedure.



MODALIZER+ can capturing video streams from Web camera and MPEG-2 or MPEG-4 video files. To start capturing, click the "Camera" button on the bottom left of the video panel.

When connected to a scanner, clicking the red capture button launches the scanner's interface. The scanned documents are added to the bottom panel of attached documents.

Click the add files button to browse for images and documents and attach them to the procedure.

You can add image comments to every image by clicking the pencil  button on every image thumbnail.

NOTE: if not edited, the comments are not inserted into the converted files.

NOTE: if user selects to build one multi-framed DICOM file - comments will be inserted into "PerFrame" sequence:

DICOM Tags			Filter by name:	x	Filter by value:	x
{0028,0100}	BitsAllocated	8				
{0028,0101}	BitsStored	8				
{0028,0102}	HighBit	7				
{0028,0103}	PixelRepresentation	0				
{5200,9230}	PerFrameFunctionalGroupsSequence					
Item[1]						
{0020,9111}	FrameContentSequence					
Item[1]						
{0020,9158}	FrameComments	Frame 1				
Item[2]						
{0020,9111}	FrameContentSequence					
Item[1]						
{0020,9158}	FrameComments	Frame 2				
Item[3]						
{0020,9111}	FrameContentSequence					
Item[1]						
{0020,9158}	FrameComments	Frame 3				
{7FE0,0010}	PixelData	332163920				

2.3. Filling a Report

MODALIZER+ is a great reporting tool, automated, customizable, and fully integrated with your PACS and Worklist Manager.

MODALIZER+ Formatted Report automatically fills patient and study information into report templates. The report templates are customizable. You can add your own logo and signature, and use your own stationery style.



There are three ways to create a report in the acquisition screen:

1. Formatted Report - to create a new PDF using the predefined formatted report templates, select the template from the list, and click the “Formatted Report” button – this will create a new file from the template. Edit and save it as PDF. Close the editor. Verify that the PDF file was added in the bottom panel.
2. Attach an existing PDF file from your computer: select a PDF file using the “Add files” button or drag-and-drop the files on the Acquisition screen.
3. Create a DICOM Structured Report by typing text in the report text panel.

Note: For more details on this feature read the [Reporting chapter](#).

2.4. Export DICOM Removable Media (CD/DVD/USB)

To complete this task, please verify that you have a CD/DVD Writer in your computer. If you don't have a CD/DVD Writer, you can export the study to any removable media like Disk-on-Key or to a directory on your hard disk.

Prepare the DICOM files that you would like to export.

- In the main menu click “Export”.
- Select the source folder with files to export.
- Click “Scan”. MODALIZER+ will now read the data from the files and prepare them for export. MODALIZER+ will display the study details.
- Verify that the “Copy, Arrange and Rename” option is selected.
- Checkmark “Include DICOM Viewer to DICOMDIR”.
- Select a destination folder to which MODALIZER+ will prepare the files for export.
- Click “Next”.
- Select the destination drive for the media.
- Click “Burn to disc”.
- After the operation completes, eject the disc.
- Test the disk: Insert the media. If your AutoRun option is disabled click the DICOMViewer.exe - the study will be displayed in the DICOM Viewer.

Note: For more information see [Burn CD/DVD](#).

2.5. Viewing DICOM files

To display a DICOM file simply drag-and-drop the files on the MODALIZER+ window. You can drag-and-drop one or more files, a directory or a DICOMDIR file. You can also drag-and-drop files and folders on the MODALIZER+ desktop icon.

Note: Read more about HRZ's [DICOM Viewer](#).



2.6. Connecting To PACS

Maximize your MODALIZER+ capabilities by connecting to a PACS. Once MODALIZER+ is integrated with your Storage and Worklist servers you will be able to use [Modality Worklist](#) to obtain Patient and Procedure parameters and [Query/Retrieve](#) to search for studies stored in the PACS..

Read more about [Storages Servers configuration](#) and [WorkList Servers configuration](#).

2.7. The Local Archive


MODALIZER+ has a local DICOM Archive to store the created, converted, and imported studies. All the files in the local archive are stored according to the DICOM Standard using the DICOM file format and are registered in the internal application database.

To enable the local archive open the [settings](#) screen and checkmark “Use Local Archive”.

PATIENT NAME	PATIENT ID	SEX	BIRTH DATE	ACCESSION NUMBER	STUDY DATE	STUDY DESCRIPTIO	No OF SERIES	No OF IMAGES	STATUS	INSTITUTION NAME	BODY PART EXAMINED
aaa*aa***	111			222	20200227	DICOMIZED...	1	3	New		
sdfdds*sdfdd...	3543	M	20200127	34543	20200127	DICOMIZED...	5	6	New		


3. DICOM Viewer

MODALIZER+ is a powerful and friendly Multi-Modality DICOM Viewer.

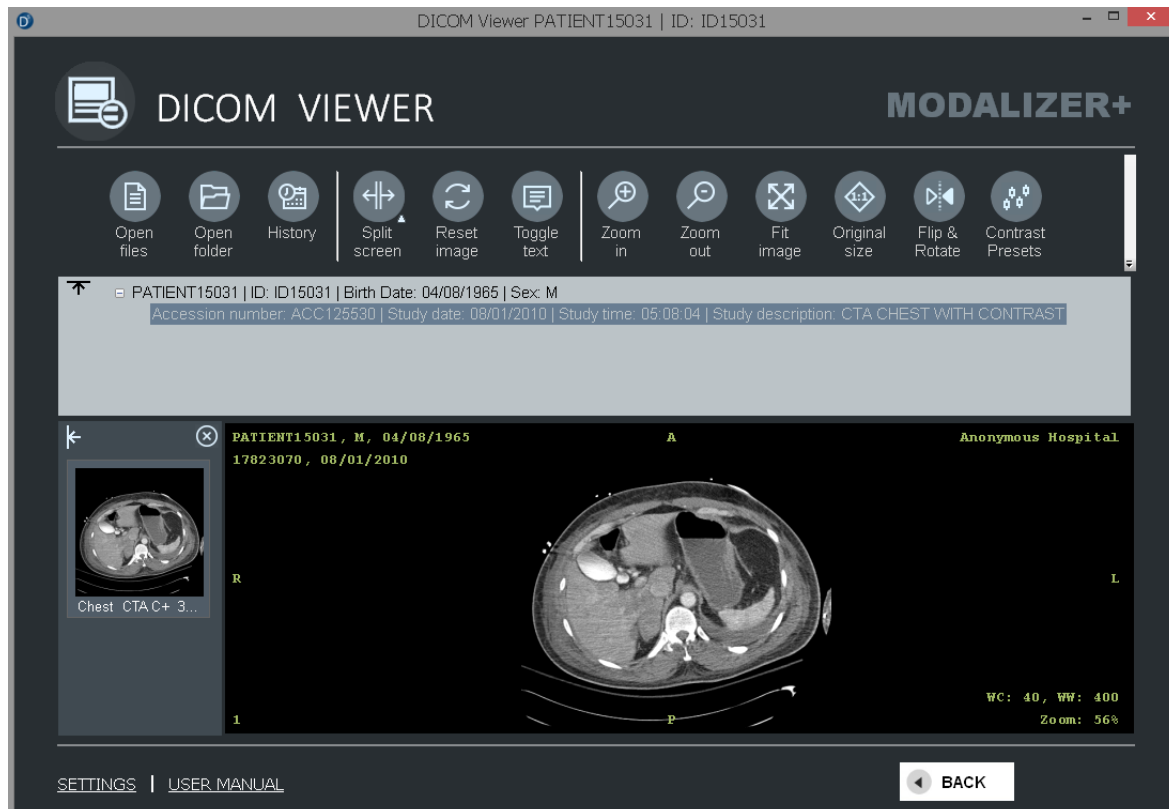

The DICOM Viewer consists of:


1. Main display area – display the selected image. Press CTRL-H to show/hide the DICOM attributes, CTRL-T to show/hide the text overlay. Right click to open the context menu with various operations, start/stop tools, open folder containing current image, send image to PACS and save it according to an original SOP class and transfer syntax (as JPEG/PNG/BMP/PDF/MPEG file). In addition each file can be saved as "Text" (DICOM dump):

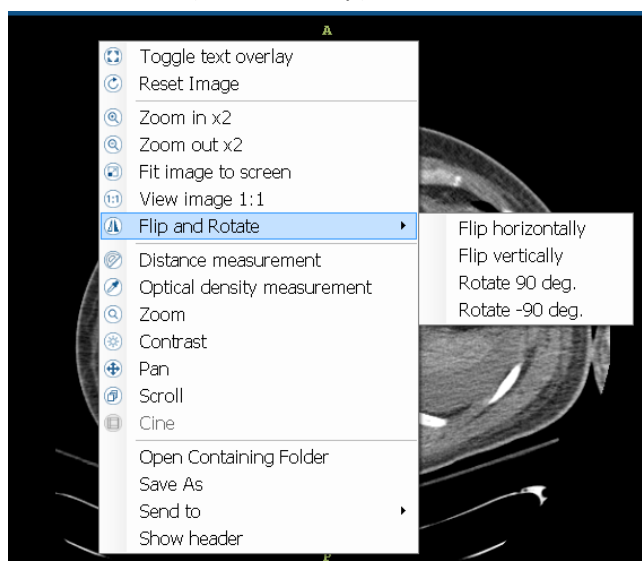



Click F11 to enter the full screen mode. In full screen mode the image display panel takes the entire screen and the other panels are hidden..


Full-screen can also be toggled from the right-click context menu and additionally can be turned off (once active) by clicking the ESC key or by clicking the 'x' button on the top-right corner:

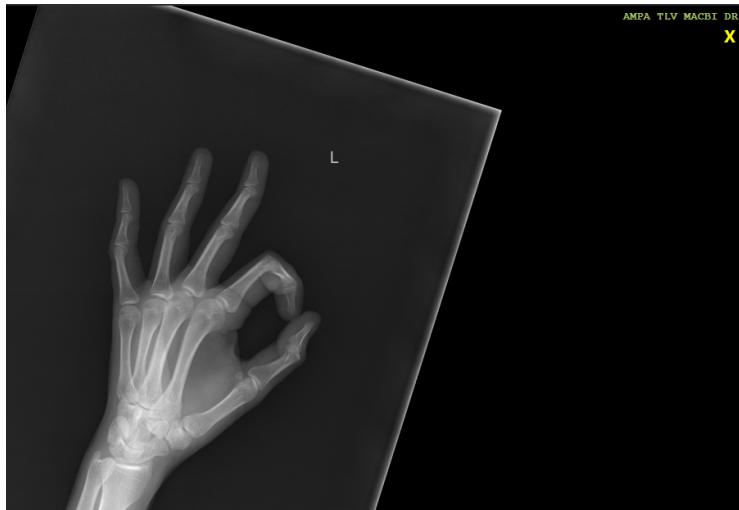

2. Patients and Studies tree –right click on the study row to show the context menu with options to send the study to PACS, close it (remove from the viewer) or export it to external media (available only for studies from Local Archive).
3. Series thumbnails of the currently selected study - right click on the thumbnail shows a context menu with an option to send the series to PACS.
4. Preview of the images within the currently selected series (as thumbnails in the bottom panel). If the images within the series are spatially related then they will be grouped and not displayed as individual files. If all the images of the current series are spatially related then no image thumbnail is displayed for the series. You can send a single image to PACS - the right click on the image opens a context menu with such an option.
On selection series first image will be displayed in central area. To display another image - click on its thumbnail or click left/right arrow to load next/previous image.
5. Tool buttons strip allowing to perform various operations on the current image and load new images from folder/file open dialog or from history record. DICOM Viewer operations can be made from the toolbar or from the context menu from right-click on the image panel.

The panels can be expanded/collapsed by clicking the arrow icons at the top left of each panel.

Right-click the toolbar area to open context menu allowing to customize the toolbar and select which groups of buttons are visible.

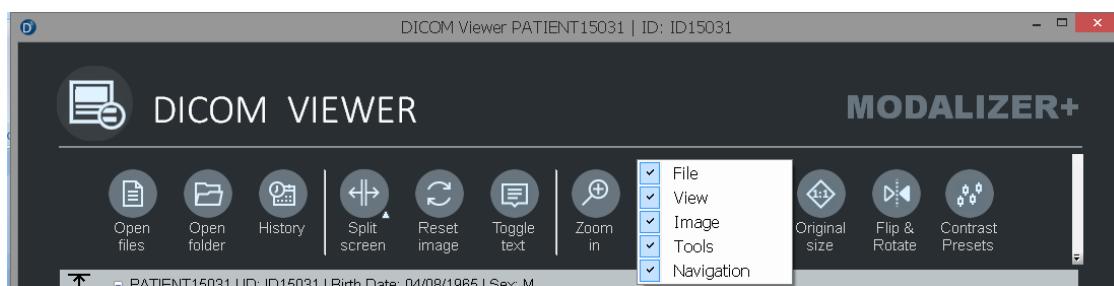


3.1. Loading images to the Viewer

There are few ways to display DICOM files - you can drag and drop the items or to click "Open Files" or use the shortcut CTRL-O to browse for a folder and select the files to view. In order to display an entire folder's content use "Open Folder" button.

There is also an option to open files from the History screen:

History screen can be opened by pressing 'History' button or by the shortcut CTRL-SHIFT-H.

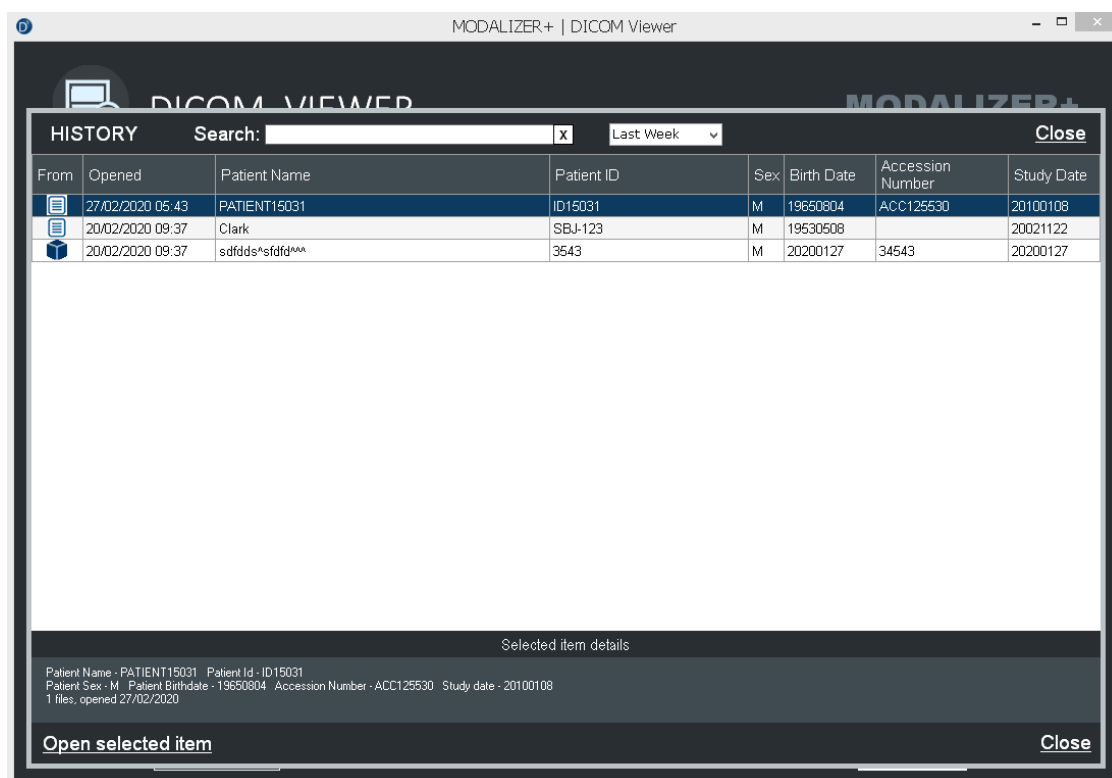


Each "open action" (Files, Folder, DICOMDIR etc.) contains one or more study rows. Study row templates is "[Patient Name],[Patient ID],[Accession Number]". To find study - type required text in the "Search" field on the top. Select entire action as shown in the image above or single study, check its details in the panel below and click "Open selected item" to load files.






If a DICOM file contains embedded video – the viewer displays it in the built-in video player (if possible), or in system Video player. Embedded PDF will be opened in system PDF viewer, SR report - in built-in HTML viewer.

Up to four (4) studies can be displayed side by side simultaneously using the split options in the toolbar.

convert

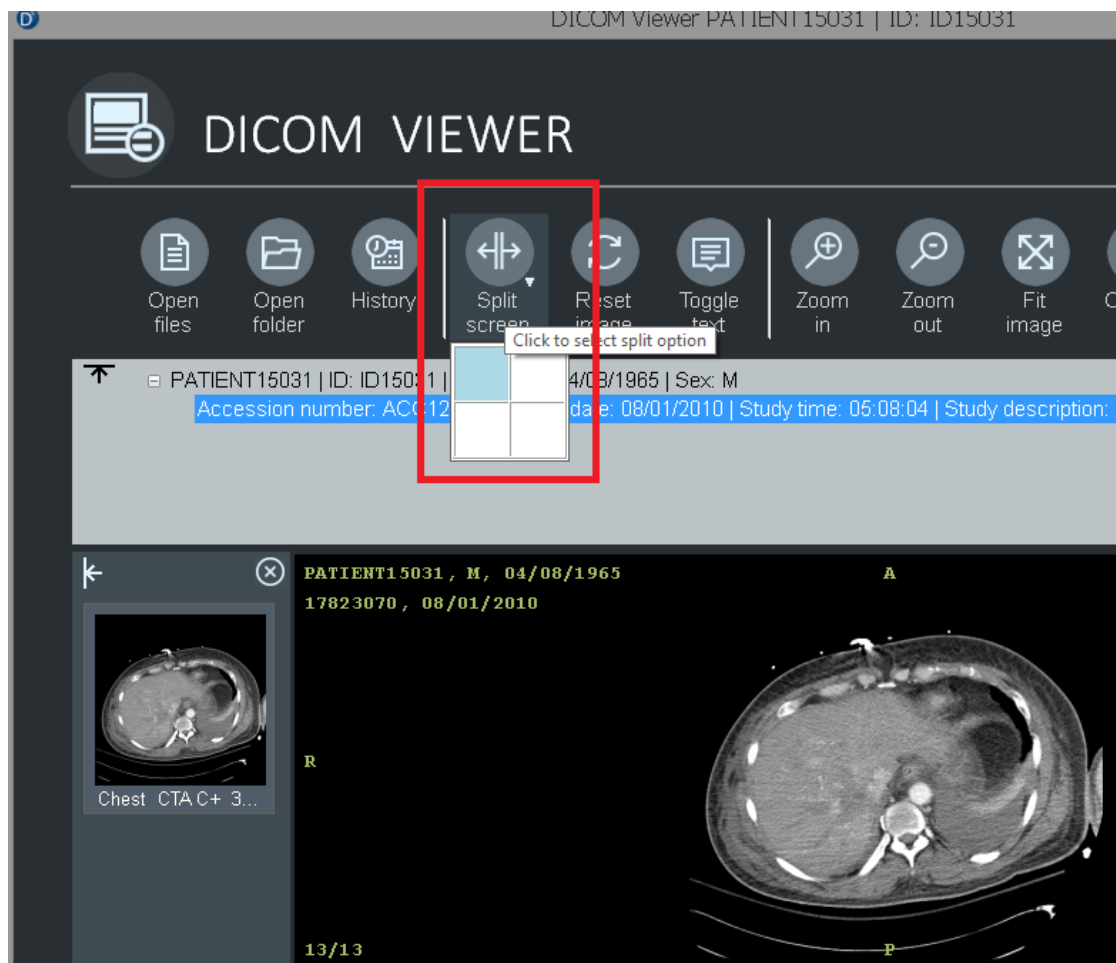


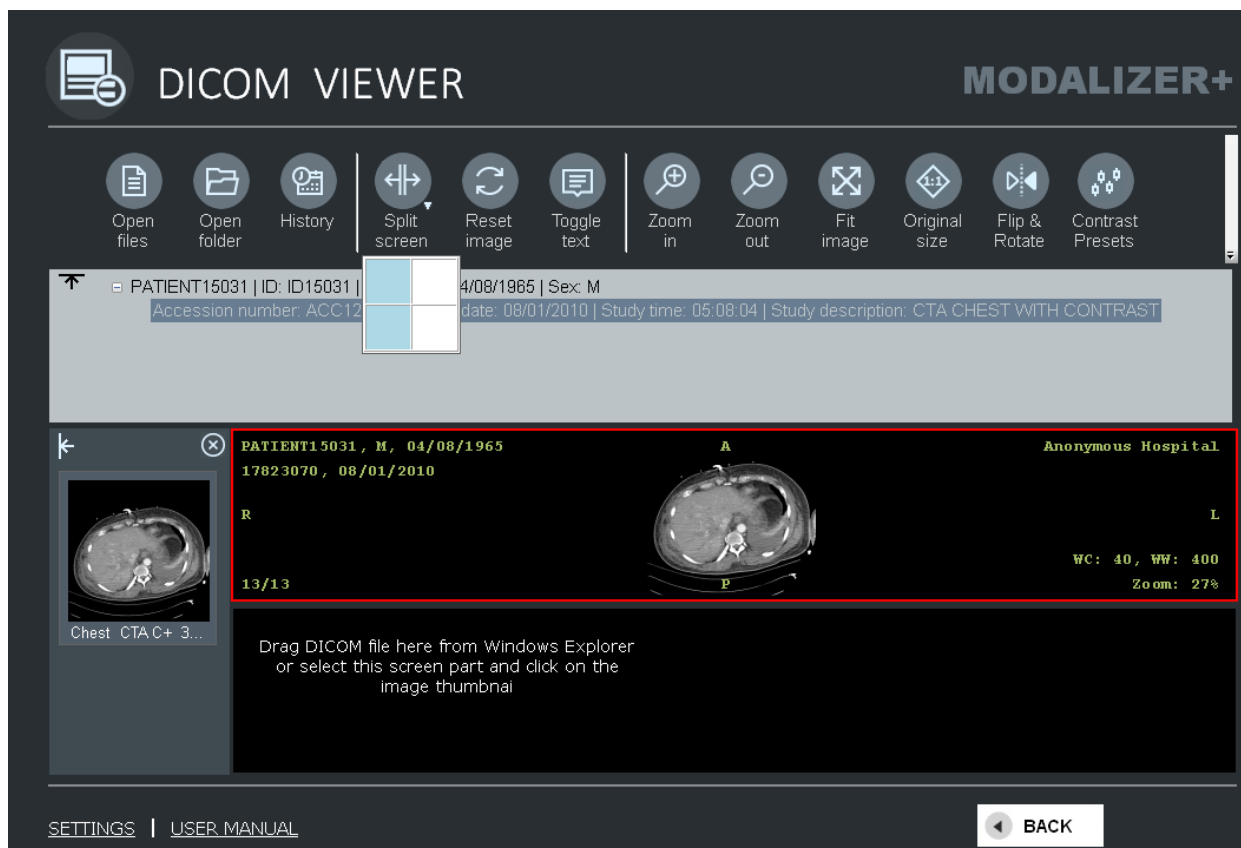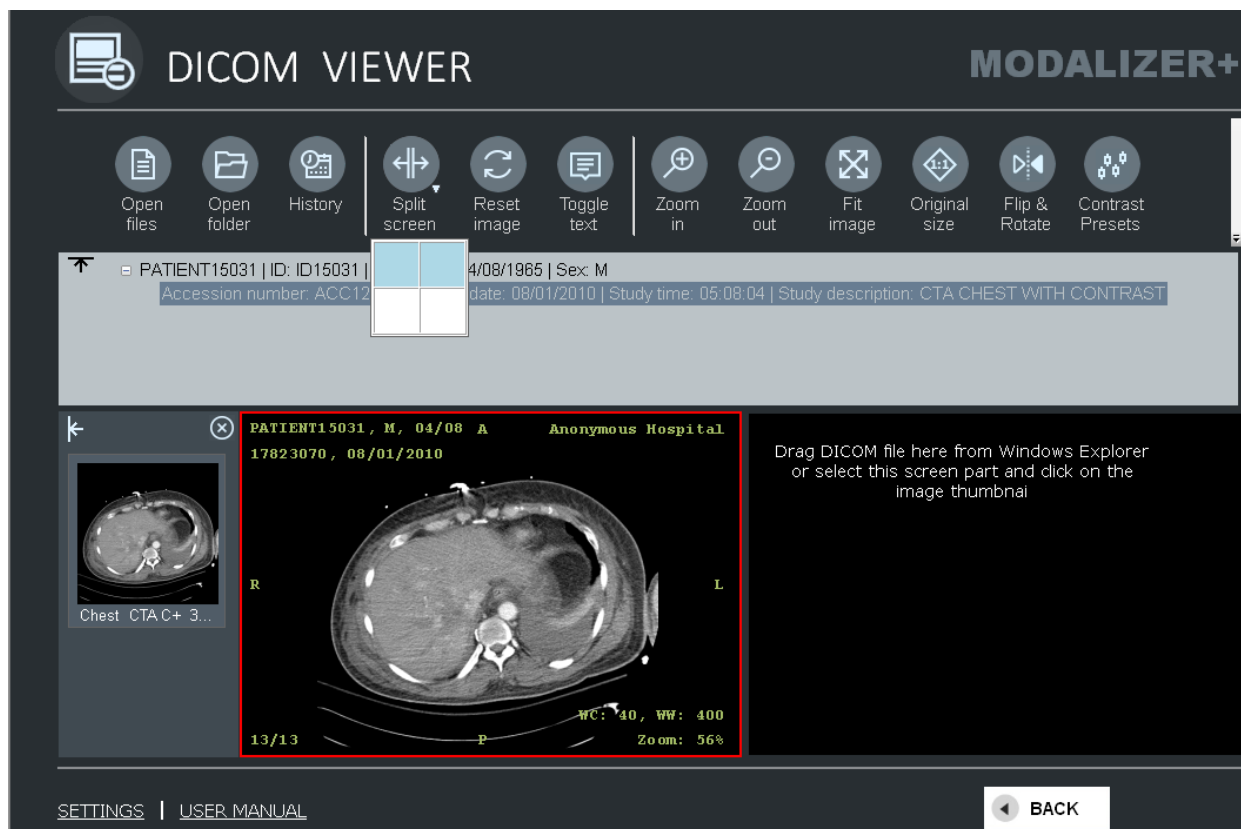


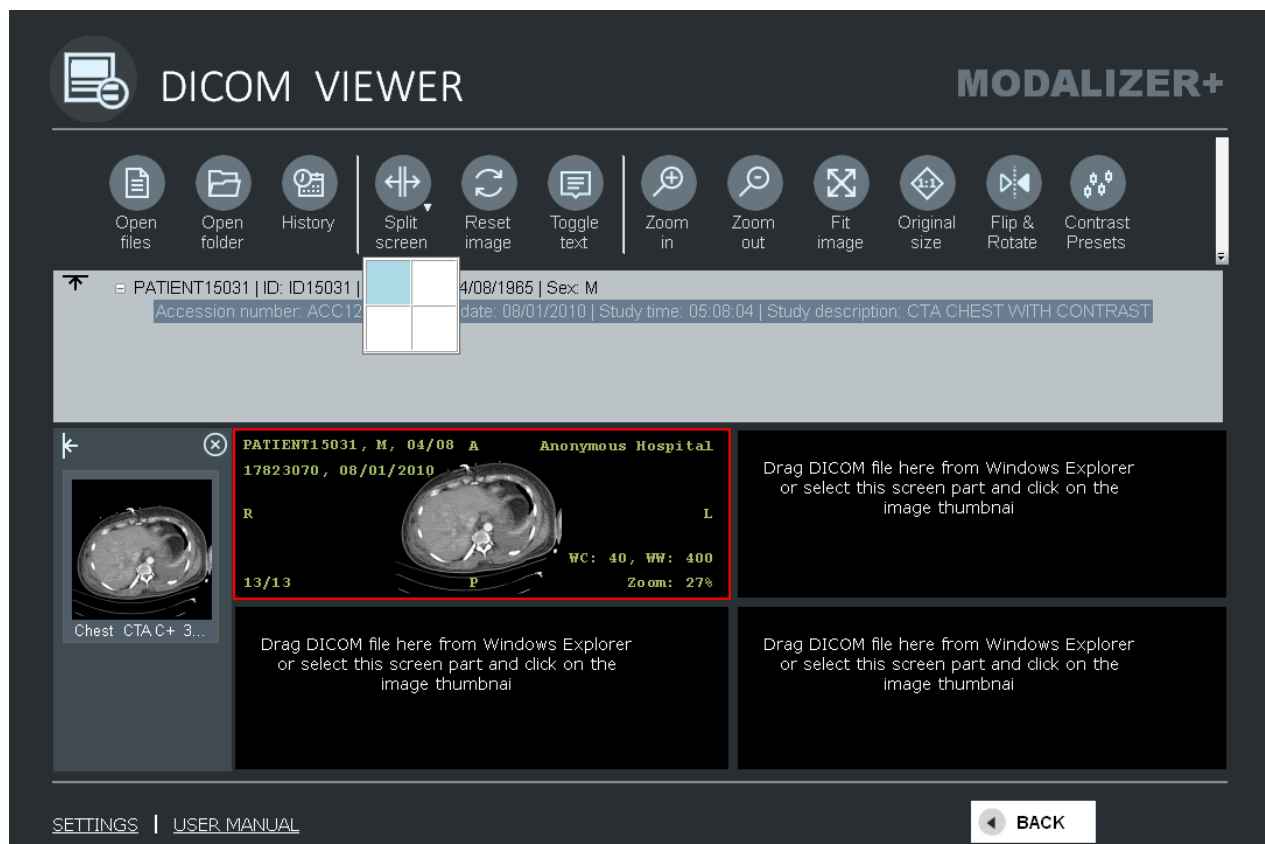

Different study might be opened in each part. To do it user needs to select required part by clicking on its area (selected part is marked by red border) and open study using usual ways ("Open files"/"Open folder"/"History" buttons). Another option is drag-drop file/folder from Windows explorer onto required part which will be selected automatically.


Clicking on each area automatically loads its study into series/images thumbnails panels:

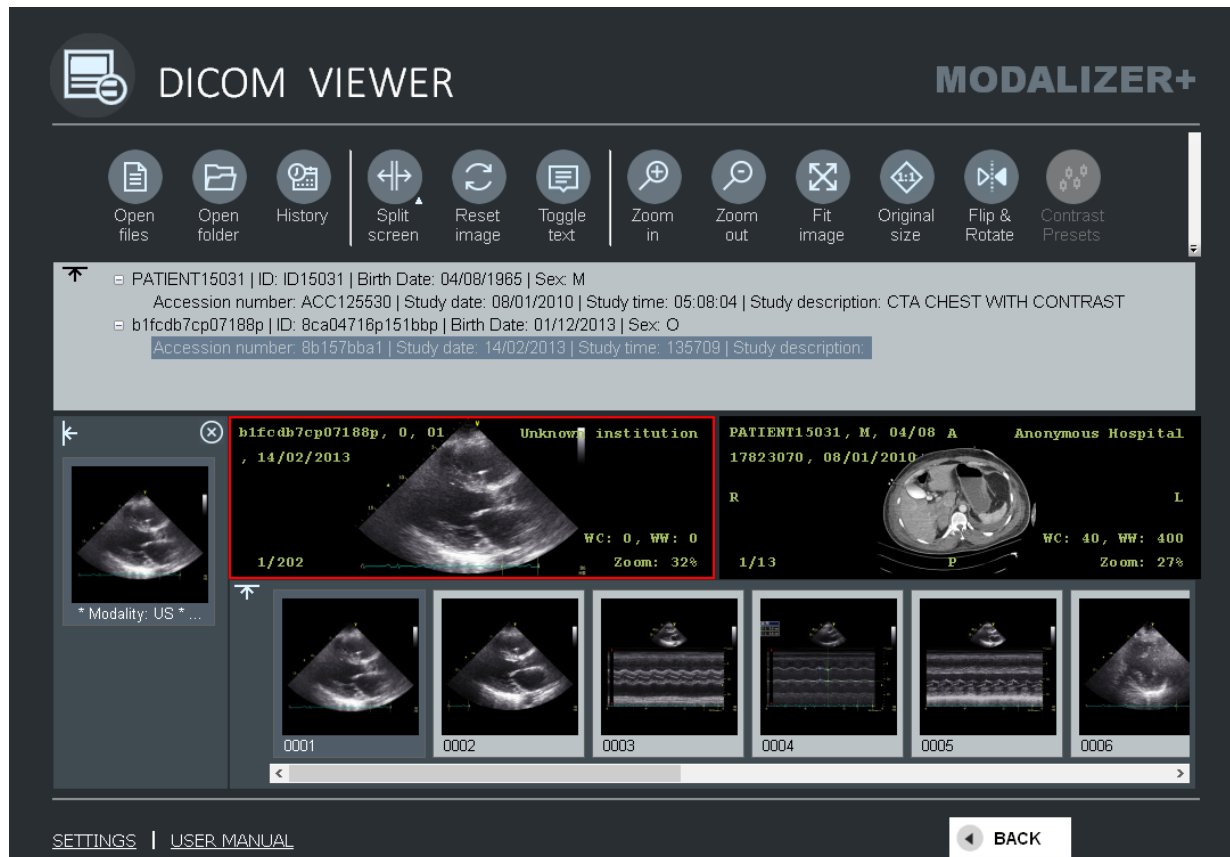

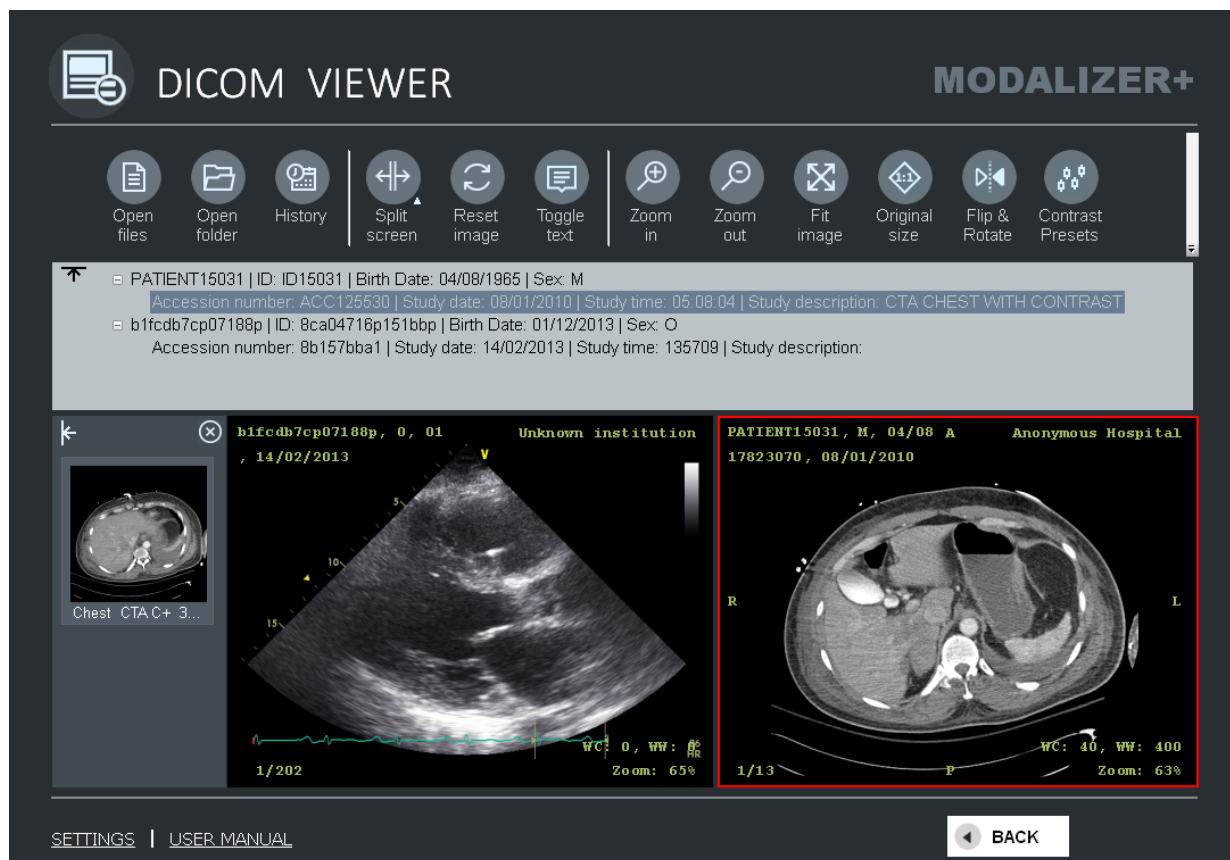

4.2. Using Hounsfield units Contrast Presets


MODALIZER+ comes with a predefined contrast presets, you can open this list by clicking "Contrast presets" tool button:

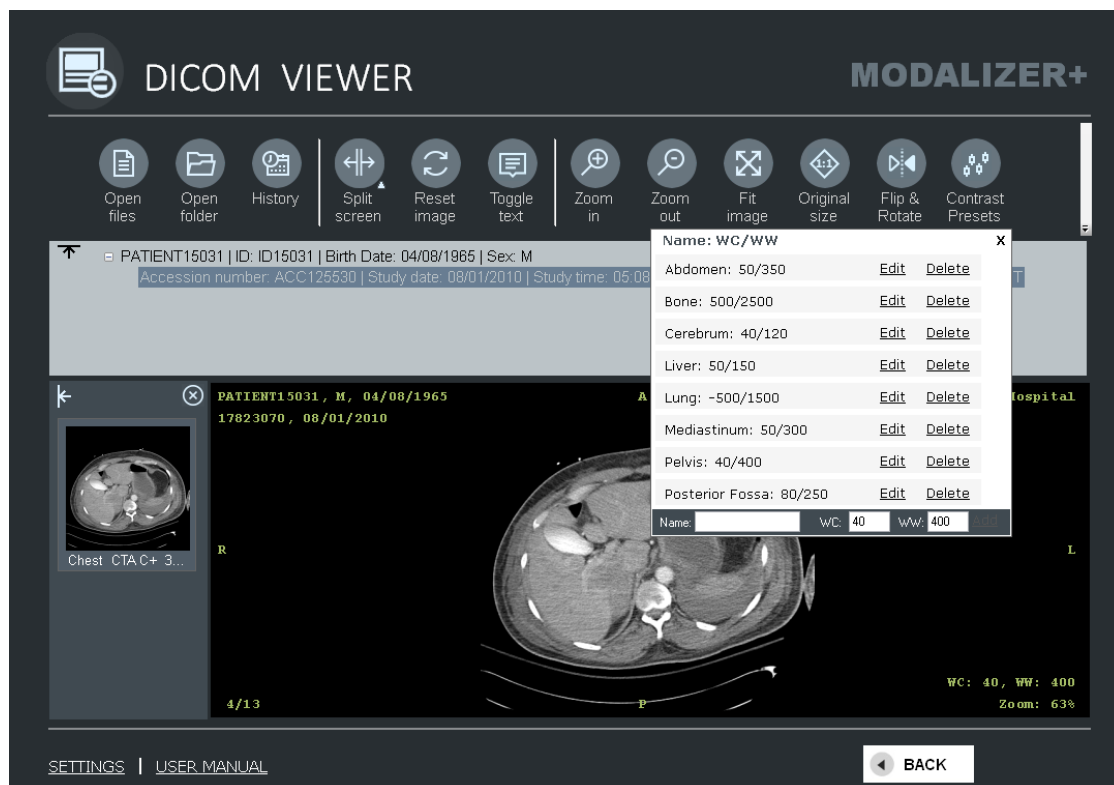

Select required presets to change WC/WW values of the currently opened image.

New custom preset can be added by filling Name/WC/WW values in the bottom line and clicking "Add" button.

You can delete existing preset or edit it in the pop-up window:

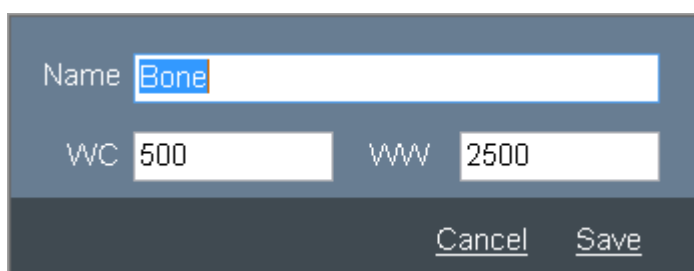

If an image contains one or more VOI LUT (Values of Interest Lookup Tables) their values will be added to the list of contrast presets.



Name: WC/WW X


VOI LUT 1 - no explanation		
Abdomen: 50/350	Edit	Delete
Bone: 500/2500	Edit	Delete
Cerebrum: 40/120	Edit	Delete
Liver: 50/150	Edit	Delete
Lung: -500/1500	Edit	Delete
Mediastinum: 50/300	Edit	Delete
Pelvis: 40/400	Edit	Delete
Posterior Fossa: 80/250	Edit	Delete

Name: WC: WW:

When opening an image with VOI LUT the first pair is automatically applied.

4.3. Distance /Optical Density / Angle Measurements tools


You can measure distance on the image (in mm for calibrated images, in pixels for others), calculate optical density in any selected point (for CT images) and measure angle between three points. To start drawing/moving click on "Distance"/"Optical Density" / "Angle" tool button:

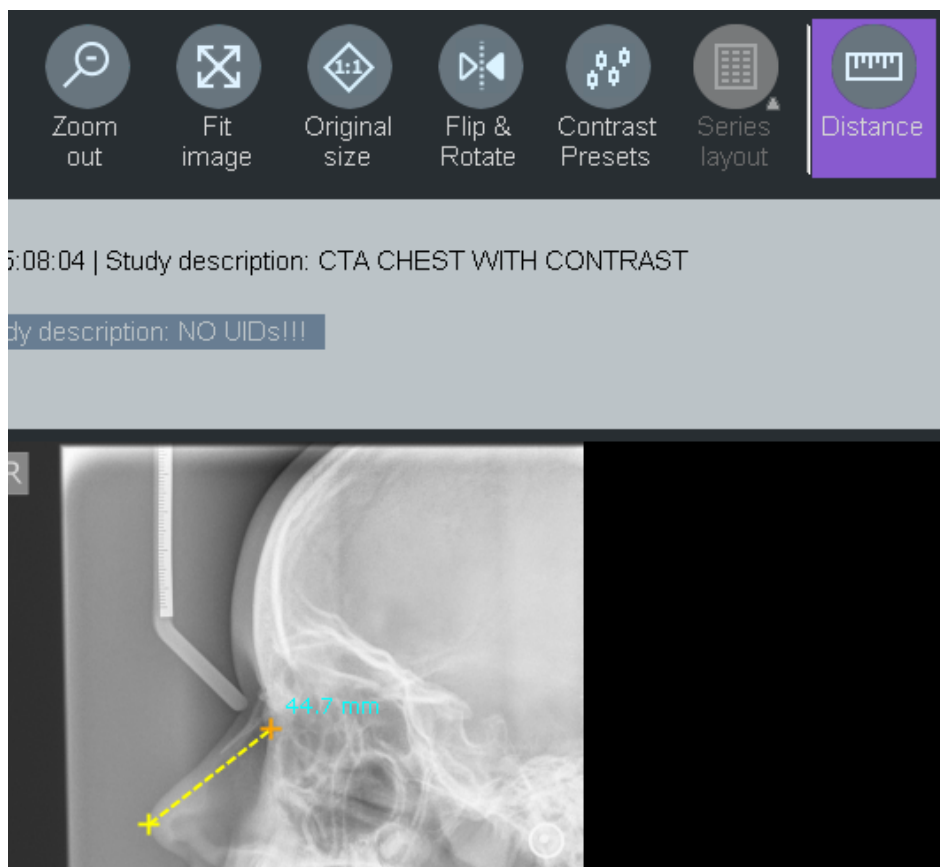


To exit the tool click on the button again. If measurement tool is not active, all existing measurements remain visible but you cannot move or delete them.

To start "Distance" drawing, click the left mouse button within the image panel. Start point will be marked as cross and dashed line will appear. Move mouse pointer to another place and left-click again to mark end point. Measured distance will be displayed on mouse move.

To start "Angle" drawing, click the left mouse button within the image panel. Start point will be marked as cross and dashed line will appear. Move mouse pointer to another place and left-click again to mark second (angle peak) point, repeat this to define end point. Measured angle will be displayed on mouse move (after peak point was created)

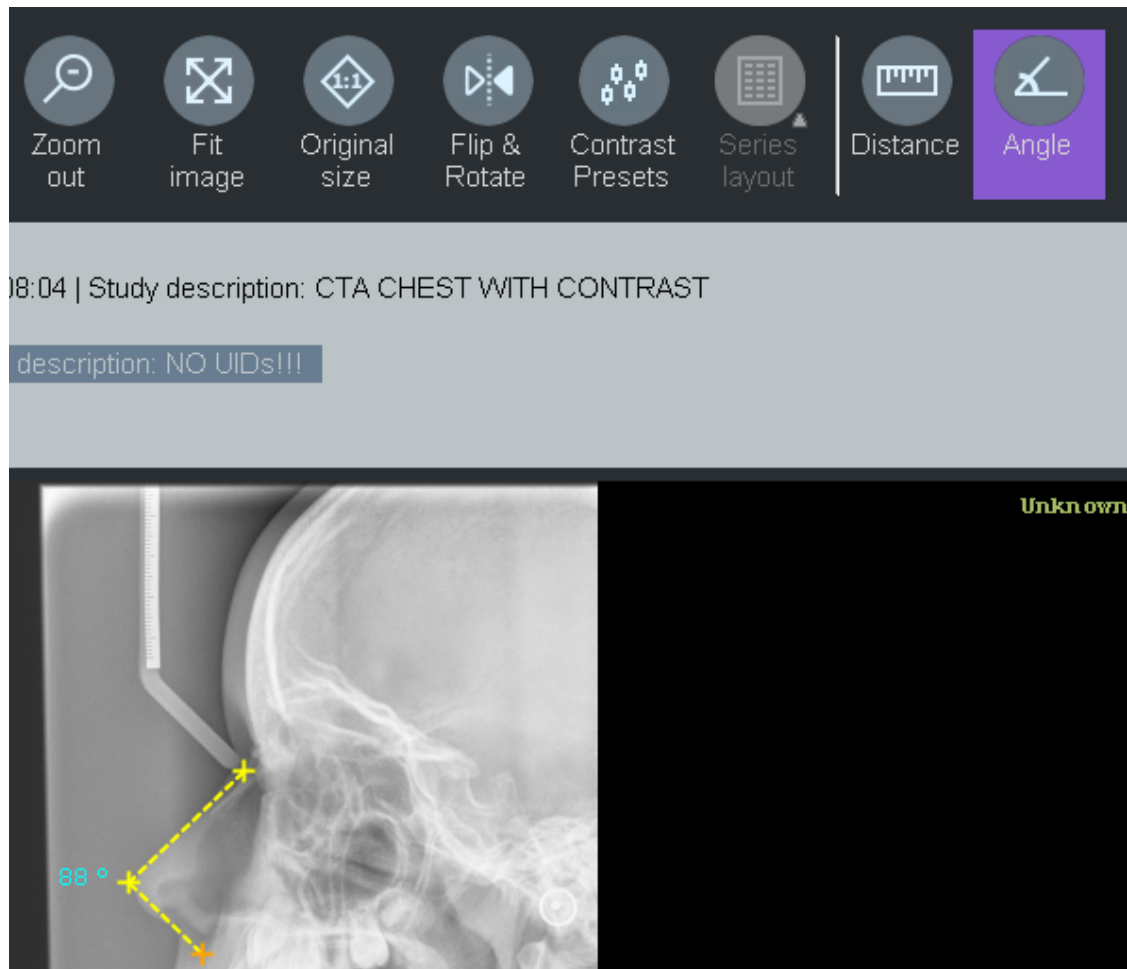


To calculate optical density click left mouse button once on the selected spot:

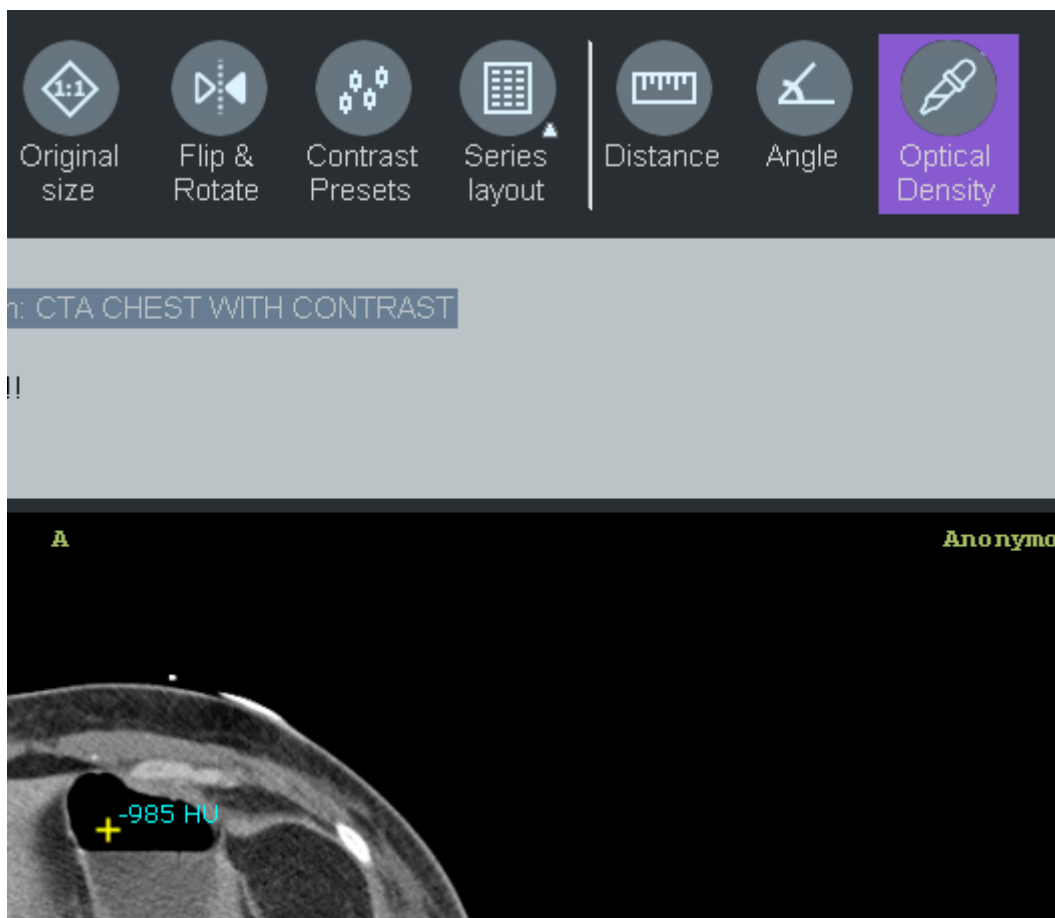

To change an existing measurement, select start/end cross or entire line (enter mouse pointer), press mouse left button and move pointer holding left-button pressed to required place and release mouse.

To delete a distance line select any part of the line and click on "Delete" button on the keyboard. You can save measurement lines / point as Grayscale Softcopy Presentation State module file under a new series (about viewing of GSPS modules - see 4.7). When user closes a study, returns from Viewer screen or exits application, and there are one or more new distance measurements, one of the following pop-up screens will be displayed:




Study has unsaved measurements

Patient Name: CARDIOART, ID : 001co
Study date: 20140303, description:

- ☐ Add entire study to local archive
- ☐ Send to: Default PACS [PACS, localhost:104]
Entire study will be sent
- ☐ Save in: ...
(if destination is empty - files will be saved in study folder)
- ☐ Don't save

OK

(Opened study is not part of LocalArchive)




Study has unsaved measurements

Patient Name: aaa^ffff, ID : ryrtyr
Study date: 20160710, description: fgnfghfghfg

- ☒ Add new GSPS module/edited files to local archive
- ☐ Send to: Default PACS [PACS, localhost:104]
Entire study will be sent
- ☐ Save in: ...
(if destination is empty - files will be saved in study folder)
- ☐ Don't save

OK

(Opened study is part of LocalArchive)

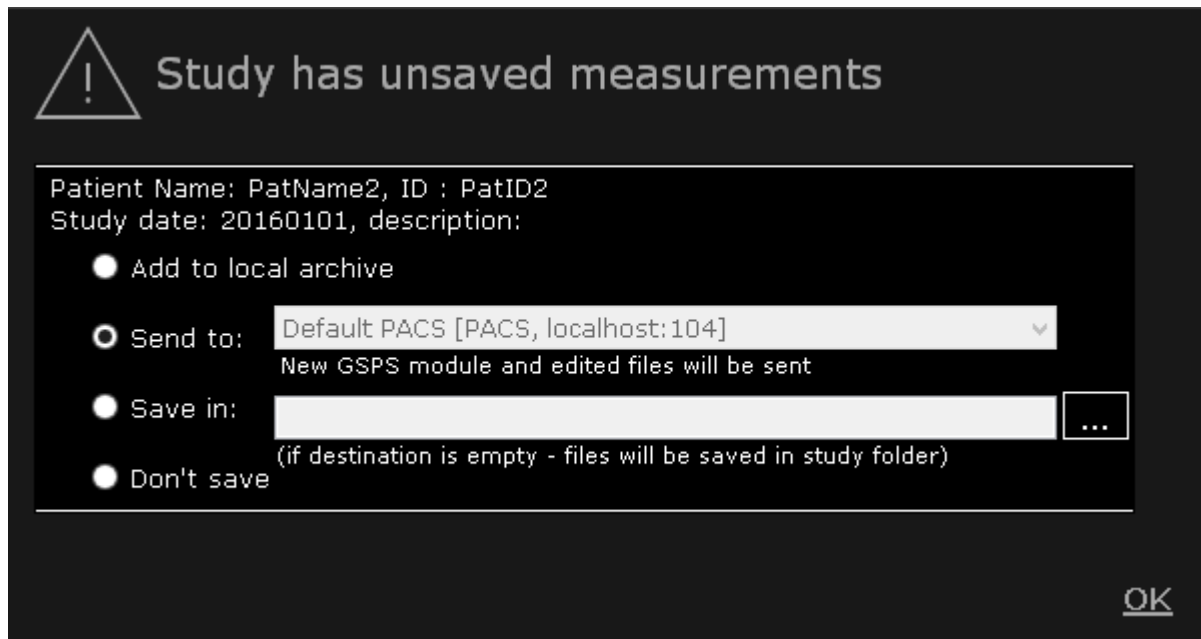


(Opened study was retrieved from PACS)

1. Select "Add entire study to local archive" to insert new GSPS file and all other files of the study into Local Archive. This option is available only if "Use local archive" was selected on the General Settings. If a study with the measurement is already a part of the Local Archive - only the new GSPS file will be added
2. Select "Send to" option to send an entire study or only new files to PACS (if a study was retrieved from PACS, source PACS will be selected by application).
3. Select "Save in" to store new GSPS file in selected folder.
4. Select "Don't save" if you don't want to add GSPS file to the study




4.4. ECG Viewer

MODALIZER+ can display DICOM 12 Lead ECG Instances.

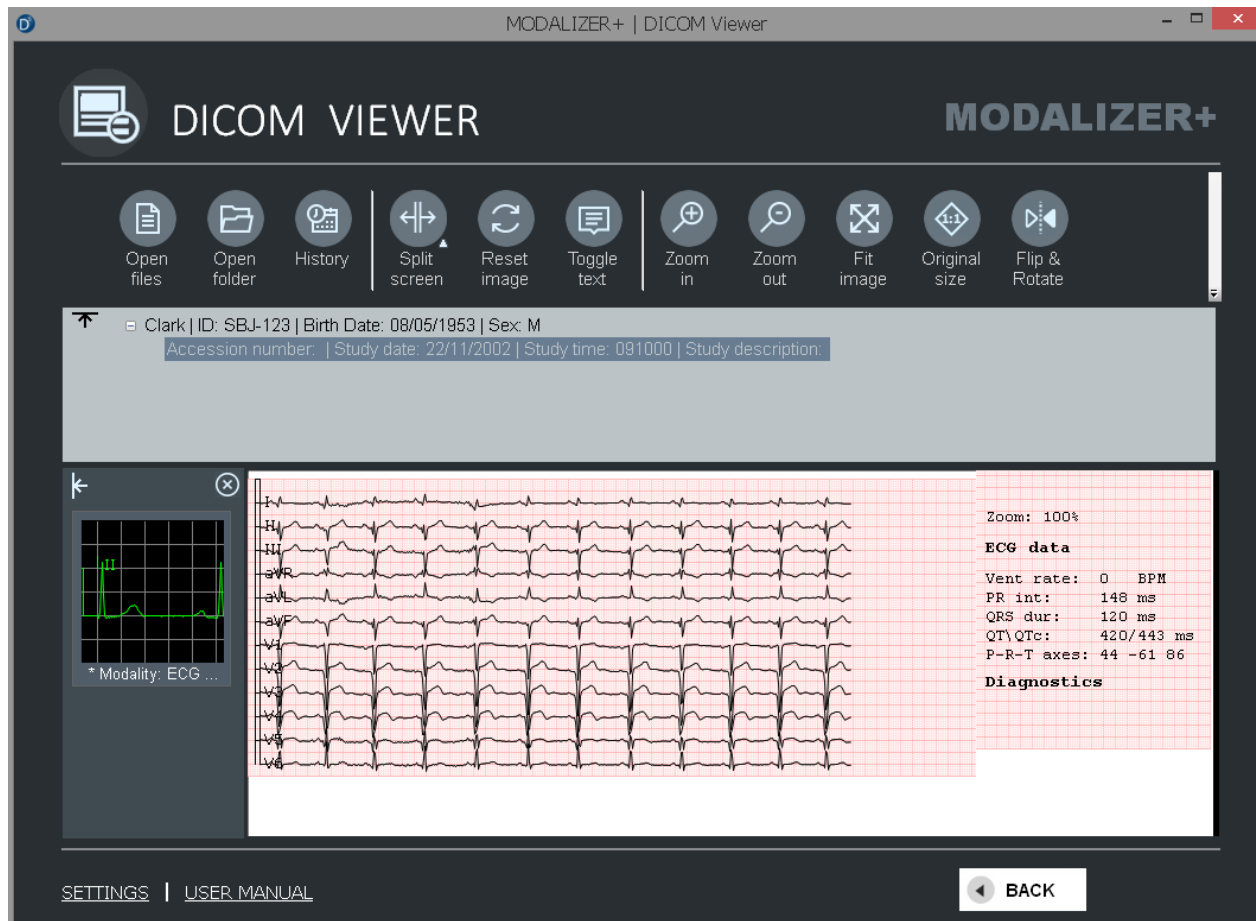


Use the ECG Display Settings tab in the configuration screen to select the graph formats (click "Setting" button from the Viewer, select required parameters and click "Back" on Settings screen. New display parameters are immediately applied.

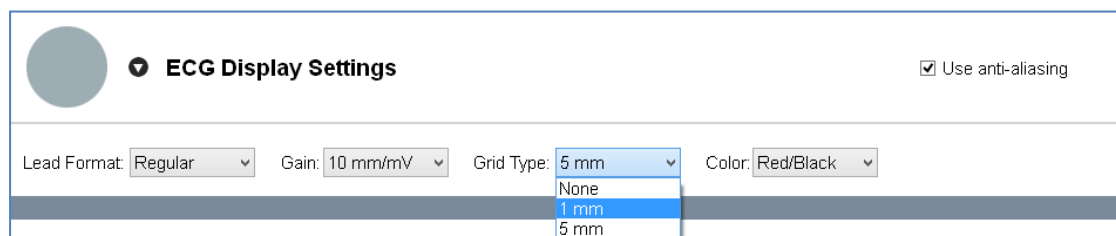

4.5. Using Zoom/Pan/Contrast/Scroll tools

To start/stop any of these tools click the tool button. When the tool is active the button background is set to red and the mouse pointer changes to the tool mouse icon:

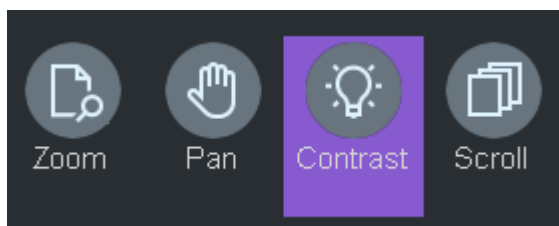


To change image zoom/contrast, move zoomed image inside viewer panel (Pan Tool) or scroll frames - press left mouse button and move pointer holding left button pressed.


4.6. Flip and Rotate tool

Available actions: Flip Vertically, Flip Horizontally, Rotate 90 Clockwise, Rotate 90 Counterclockwise. All measurements on the current image will be changed accordingly

Before:

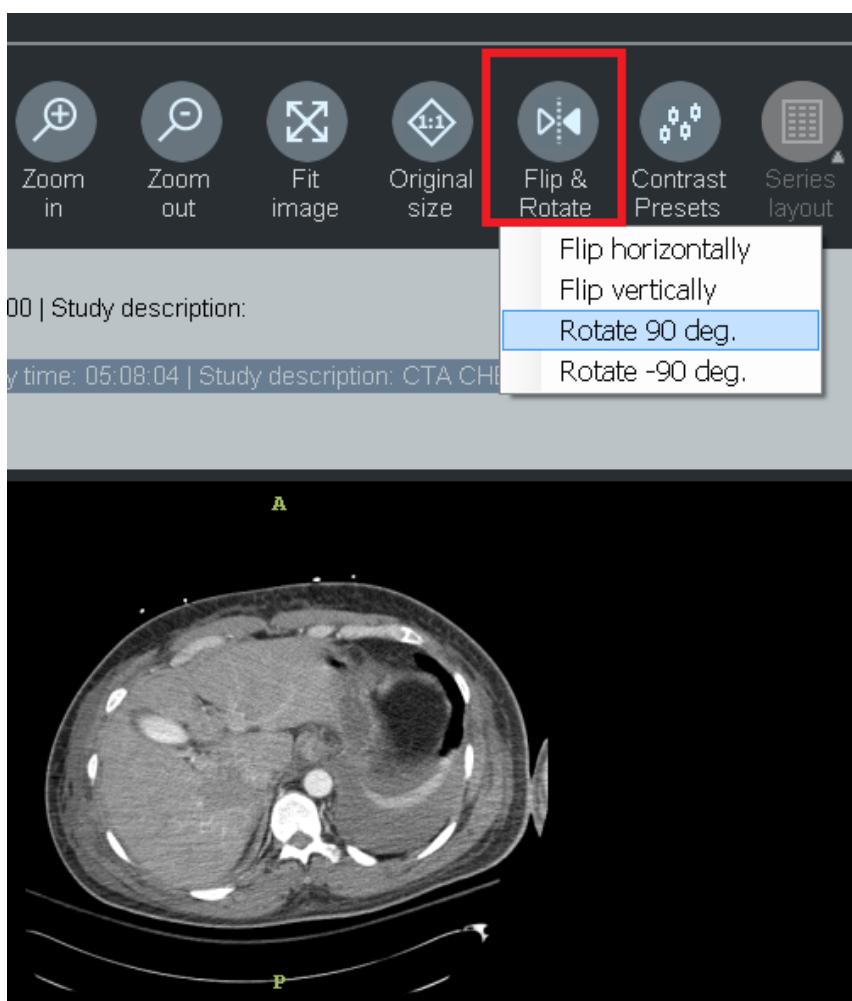



After:

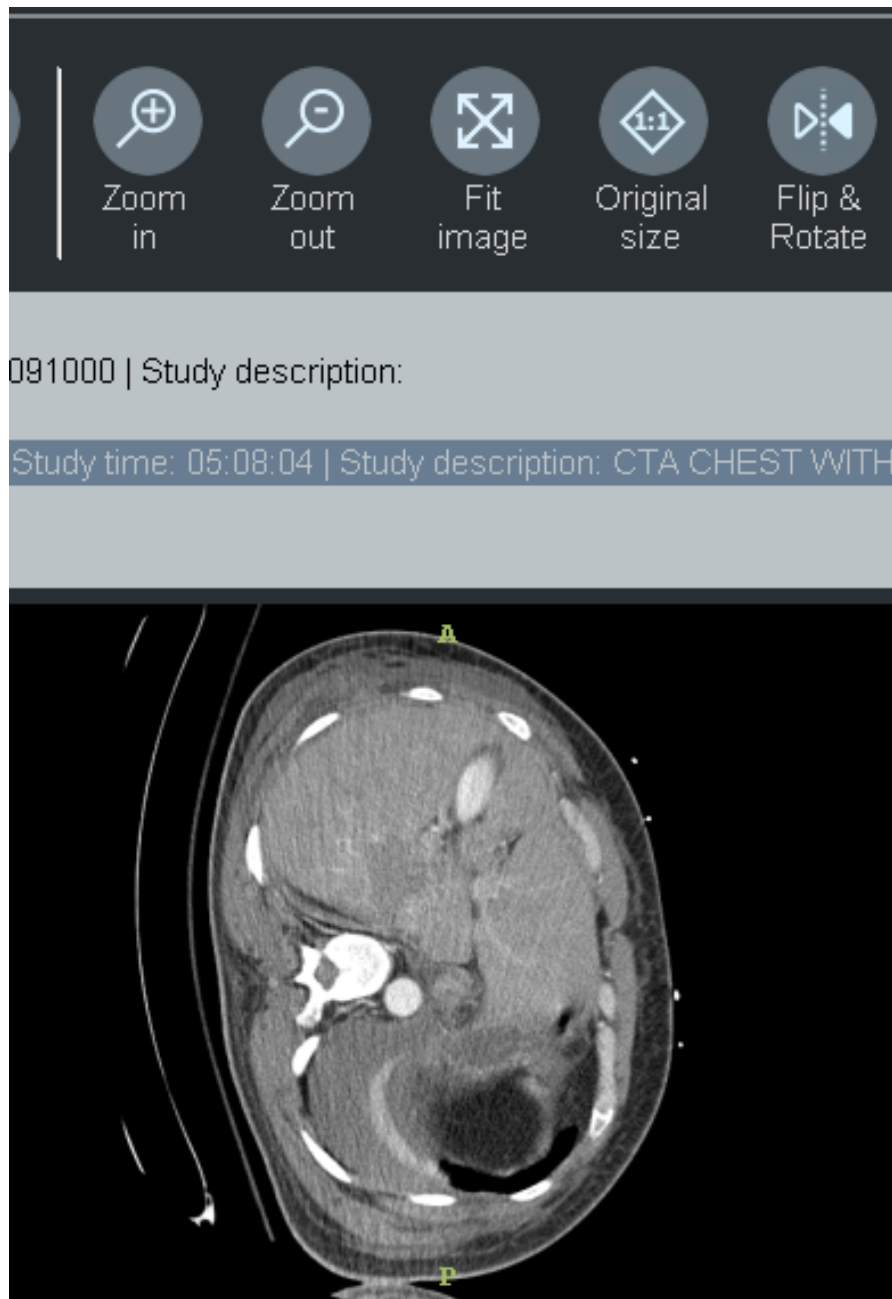



4.7. CINE tool

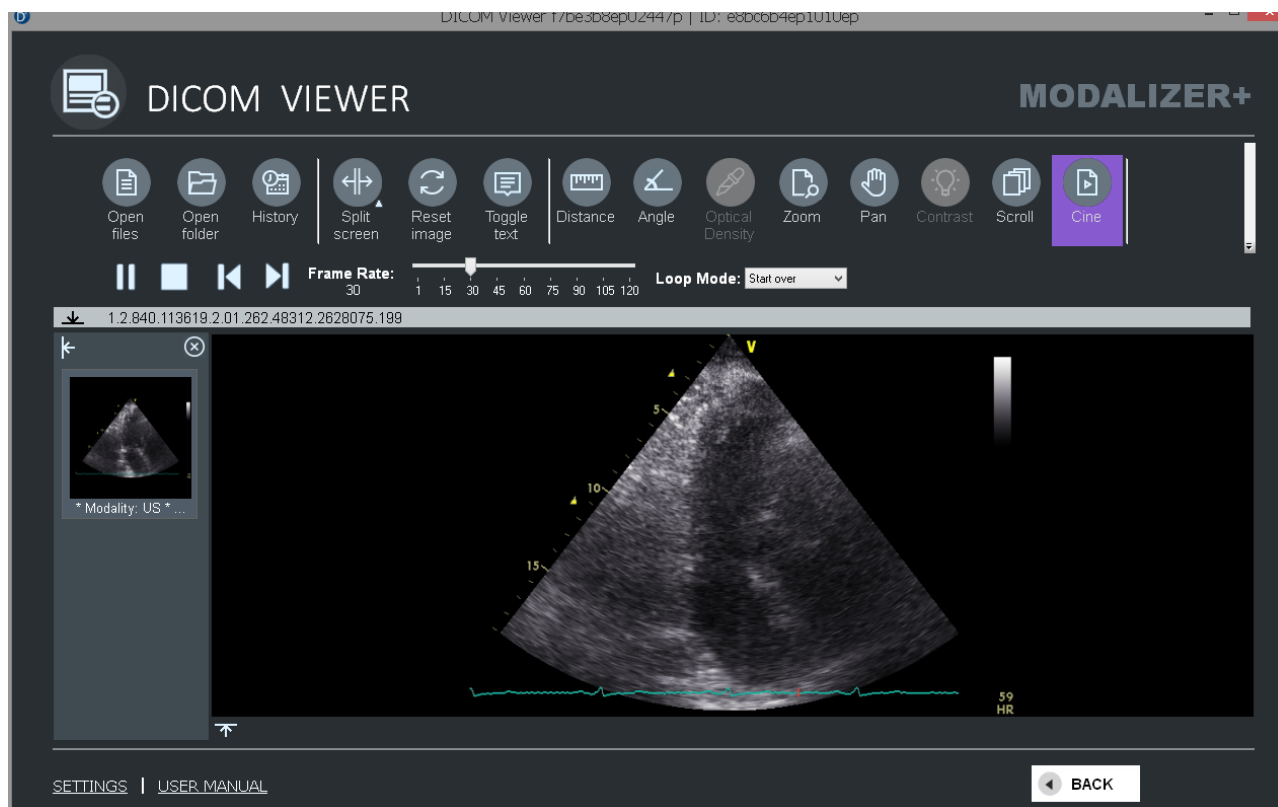If DICOM file contains multi-frame image CINE mode is enabled and the cine buttons can be used.




To Pause/Start CINE - click  button.

To Stop CINE and close CINE panel - click  button

To go to the first/last frame - click  buttons

You can change CINE frame rate and loop mode:





4.8. Display Grayscale Softcopy Presentation State module

MODALIZER+ can display graphic and text annotations stored in DICOM Presentation State objects (GSPS). When a user opens a study, the application selects all such files, loads their data (relations between annotations and study instances/frames, annotations types/positions etc.) and converts it to graphic objects drawn on the corresponding images.

Every GSPS module (series with PR modality) is displayed as a separate thumbnail in the left panel like any other series.

When a user clicks a PR series thumbnail is highlighted, the graphic objects in the GSPS module are displayed as separate image thumbnails in the bottom panel and first of them is displayed in the main area on the image and frame it is referencing.

Click on each image thumbnail loads corresponding image/frame and graphic objects into main area.

When user clicks a non-PR series (images), the annotations are hidden.

When the PR series is selected and user chooses "Show header" - the tags of the PR are displayed ("Edit" for PR files is not allowed)

4.9. The DICOM Header view (editing DICOM objects)

To view all tags containing in the current DICOM file - right-click on the image and select "Show header" or press Ctrl-H.

Hierarchical tree view will be opened so that sequences might be opened/closed by user.



NOTE: By default all private tags are displayed with "?" name, but you have an option to use dicom.dic file (located in the installation folder) to define name of any private tag. Format of




the dicom.dic tag line is:

#	Tag	VR	Name	VM	Version
	(0027,0000)	UL	SamplePrivateGrpLength	1	RZDCX

All columns MUST be separated by "Tab".

Dicom.dic file from the installation package contains few lines as example. If you don't need them - open file in Notepad and delete unnecessary lines or just delete dicom.dic from the installation folder.

To start editing - select "Show header" and click "Edit" button:




DICOM Object Editor Screen allows user to:

- Add tags
- Add sequence
- Add sequence item
- Add/Edit/Delete tag within sequence
- Duplicate sequence item
- Remove tags
- Remove sequence item
- Change value of tags

A new instance is generated from the original and updated according to the DICOM standard:


1. New series created
2. Referenced instance sequence (0008,114A) with reference to the original series/instance inserted into the new instance

New instance will be opened for editing:

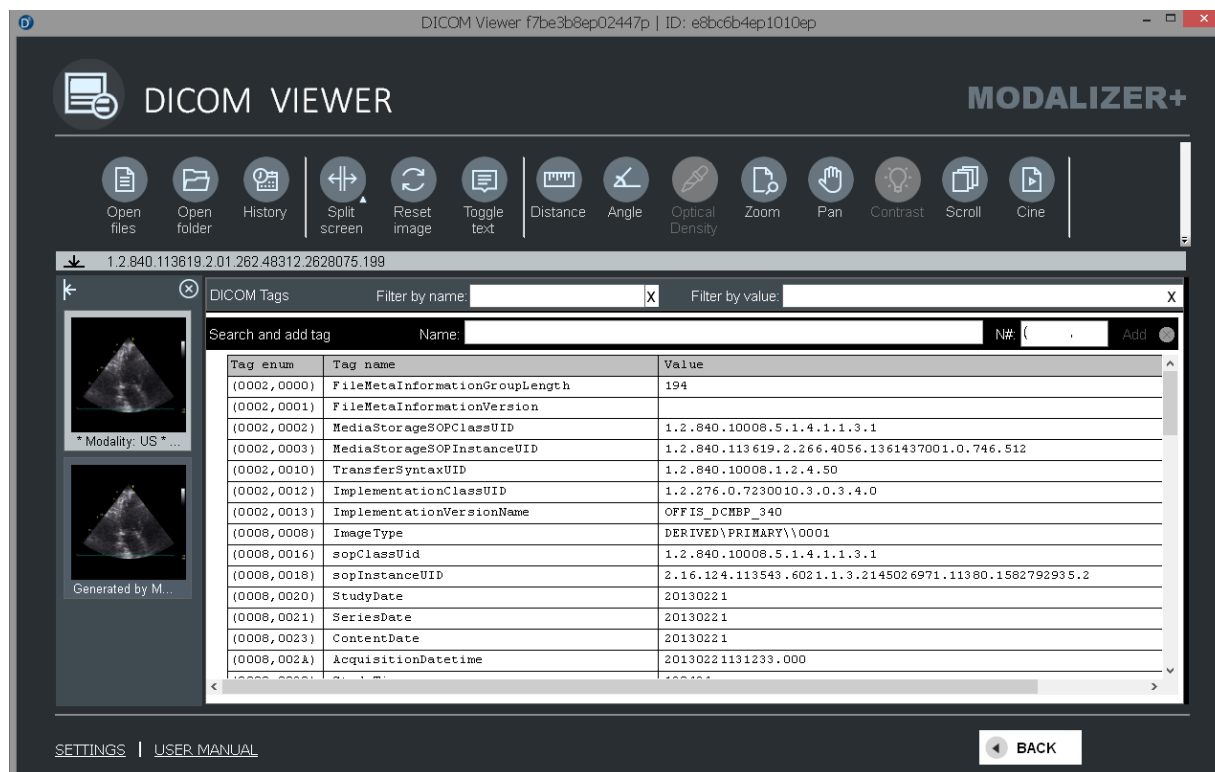

To add tag - use "Search and add tag" options. When user click "Add" button - tag will be inserted on main level or inside selected sequence

User can copy entire sequence, delete it or add tag into it. To select one of the options - right-click on sequence row to open context menu.

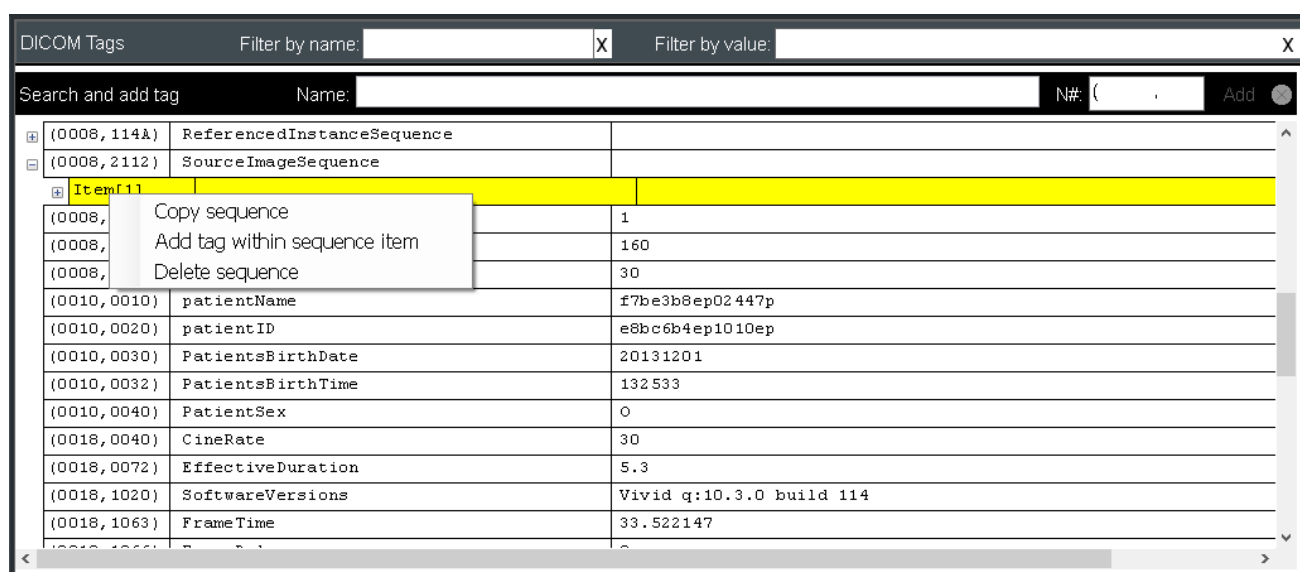



To change tag value - double-click on its row

DICOM Tags Filter by name: X Filter by value: X

Search and add tag Name: N#: (, Add

(0008, 114A)	ReferencedInstanceSequence	
(0008, 2112)	SourceImageSequence	
Item[1]		
(0008, 2142)	StartTrim	
(0008, 2143)	StopTrim	
(0008, 2144)	RecommendedDispla	
(0010, 0010)	patientName	Value: <input type="text" value="f7be3b8ep02447p"/>
(0010, 0020)	patientID	
(0010, 0030)	PatientsBirthDate	
(0010, 0032)	PatientsBirthTime	132533
(0010, 0040)	PatientSex	0
(0018, 0040)	CineRate	30
(0018, 0072)	EffectiveDuration	5.3
(0018, 1020)	SoftwareVersions	Vivid q:10.3.0 build 114
(0018, 1063)	FrameTime	33.522147

To delete tag - right-click on its row and select "Delete tag"

(0010, 0032)	PatientsBirthTime	132533
(0010, 0040)	PatientSex	0
(0018, 0040)	CineRate	30

Delete tag

On closing study user will be suggested with several option concerning new instance:

Study has edited files

Patient Name: PATIENT15031, ID : ID15031
Study date: 20100108, description: CTA CHEST WITH CONTRAST

☒ Add entire study to local archive
☒ Send to: Entire study will be sent
☐ Save in: ...
☐ Don't save (if destination is empty - files will be saved in study folder)

OK



If user decides to save new instance - Rejection Notes KOS Document will be created as new series.

4.10. Image Info View

From the context menu select “Image Info” to show the displayed image meta information (size, compression method, color space).

4.11. Shortcut keys

The following shortcut keys are available in the DICOM viewer.

Ctrl + H	Show/Hide text overlay
Ctrl + O	Open File
Ctrl+Shift+H	Show History
F11	Full screen mode
Esc	Exit full screen mode



5. Working with Studies

5.2. New Patient

Select the “New Patient” option from the main menu:

The screenshot shows the 'MODALIZER+ | New patient' window. The header includes a yellow circle icon with a person and a plus sign, the text 'NEW PATIENT', and the 'MODALIZER+' logo. The form contains the following fields and controls:

- First Name: Text input field
- Last Name: Text input field with a three-dot menu button to its right
- Patient ID: Text input field
- Patient Sex: Radio buttons for Male, Female, Other, and Not Set (selected)
- Patient Birth Date: Date picker showing 27/02/2020
- Accession Number: Text input field

At the bottom, there are links for 'SETTINGS' and 'USER MANUAL', and three buttons: 'X CANCEL', '◀ BACK', and '▶ NEXT'.

Click "..." button to show/hide Prefix, Middle Name and Suffix fields:




Enter patient's data (not required), then click "Next".

Compose the study with images and report as explained in the [Create a new Study](#) section then click "Next".

Create formatted PDF report (optionally) as explained in [Writing a Report](#)

Notes:



1. Click button  to change the style of the presentation (thumbnails/list).
2. Click on "Patient name..." strip to view full details about procedure



The “Convert” screen consists of three panels:

- Panel #1:
 - Destination Folder – where the converted files will be saved. A new directory is created in your documents folder for every conversion under the MODALIZER+ main folder. If "Use local Archive" option is selected in the Settings screen - destination folder will be created as sub-folder of storage place defined in Settings. If not - you can change destination to any folder on your computer.
 - Report Title.
 - Create report as – MODALIZER+ allows you to create a DICOM SR (default) or as an encapsulated PDF.
- Panel #2:
 - Image Format to save in DICOM:
 - “Automatic” (default) - the files will be converted to DICOM the way they are. JPEG Images will be converted as JPEG and other as uncompressed.
 - “Uncompressed” - all files will be first uncompressed and converted to DICOM.¹
 - J2K - Convert all images to Jpeg 2000

¹ Changing the image format may result in quality loss.



- “JPEG” - all Images will be converted to JPEG as Encapsulated JPEG using the JPEG Lossy Transfer Syntax.²³
- Create one Multi-Frame File – use this option when you have a series of related images. All images must be the same format and the same size.
- Panel #3:
 - Convert - converting only. The converted files will be saved in the destination folder.
 - Convert and create DicomDIR. DicomDIR is a file that includes patient and study information and links to all the converted files.
 - Convert and send to PACS. In order to save the study on PACS you need to configure it. See [Storage Server configuration](#).

5.3. Sending DICOM Images to the PACS

DICOM files are typically stored in a PACS. This allows accessing them from other DICOM applications.

After acquiring the study images the “Convert” screen is displayed. Select an option “Convert and send to PACS”. If a PACS wasn’t defined yet click “[Settings](#)” and configure it. Then click “Next”.

Click “Send to”.

[How to send the same study to multiple destinations](#)

² Some PACS May not allow storing JPEG Compressed DICOM Images.

³ JPEG Compressed Images usually take less disk space and may be faster to store and restore from the PACS but lose some quality compared to uncompressed files..



5.4. Modality Worklist Query

In order to use the Modality Worklist Service configure a [Worklist Server](#).

Click “Modality Worklist” in the main menu:

The basic search is done by the patient name or by patient ID. If you are not sure in patient’s name spelling you can use wildcard characters “?” and “*”. “?” is used to represent a single character and “*” represents any number of characters. Click “Advanced Search” to present additional search options like a range of days when the study has been created or by the accession number. Clicking “Search” with no search parameter set will list all the existing studies. This is not recommended and it may take a very long time.

Search also can be started by pressing "Enter" in any text box in the Advanced Search area.

A default search filter can be set in the settings screen for “today” and for a specific scheduled AE title. To enable this mark the appropriate check-boxes in the [“Worklist Server”](#) settings panel.



On screen opening query will be sent to the default MWL server (one currently selected in the settings screen) but you can switch to another server by selecting it from the list located under search panel.

MODALIZER+ uses the attributes received from the MWL Query in the new study Images and report.

Double click on the row from the list of results or clicking the "Next" button will lead you to document the study by creating images and [adding a report](#).

NOTE: If "Two step verification" option on the "Worklist Servers" section of the settings screen is selected - all the data from the selected MWL entry will be displayed in a popup modal windows before starting the procedure:


The screenshot displays the MODALIZER+ Modality Worklist interface. A modal window titled "Full Procedure Info" is open, showing the following fields:

- Patient name: test*test
- Patient ID: 1313321
- Patient sex: O
- Patient birthdate: 27/02/2020
- Requested Procedure Description: Tests
- Accession Number: 200227113414365
- Modality: OT
- Station Name: test
- Referring Physician Name: test
- Procedure Start Date: 27/02/2020
- Procedure Start Time: 11:34:00
- Scheduled Procedure Step Description: test

At the bottom of the modal, there are two buttons: "Start procedure" and "Cancel".

The background interface shows a list of worklist items on the left and a top navigation bar with "MODALITY WORKLIST" and "MODALIZER+" labels. At the bottom of the main window, there are buttons for "SETTINGS", "USER MANUAL", "CANCEL", "BACK", and "NEXT".

Right click on the row opens menu allowing to copy/print patient and study info or execute some custom action using selected data ("test" in the below image):

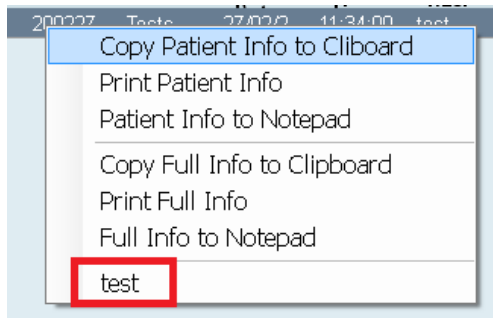

[How to configure Customs Actions.](#)

5.5. Query/Retrieve - Searching the PACS

Query/Retrieve (Q/R) is a DICOM Service that allows to search for DICOM objects in a PACS using search criteria (patient name, date of creation of the images, modality etc.) and retrieve them for viewing or other purposes. To use Q/R you configure a [Storage Server](#).

Select "Query Retrieve" from the main screen.

MODALIZER+ | Query Retrieve | DSR SVC

QUERY RETRIEVE

Advanced Search [SEARCH](#)

Patient name: Accession number:

Patient ID: Study date: ☒

Patient birth date: ☐ Study from: ☐ To: ☐

Patient Sex: Modalities in study: [CLEAR](#) [SEARCH](#)

Destination Folder:

Studies list (to retrieve selected study double-click on the row or select row in the grid and click "Next")

Patient Name	Patient ID	Birth Date	Sex	Study ID	Study Date	Study Time	Mod.In Study	Acc#	Ref. Phys. Name	#Series	#Inst	Study Instance UID
aaa*aa...	111			1	202002...	111558...	OT	222		1	3	2.16.12...

[SETTINGS](#) | [USER MANUAL](#)

X CANCEL ◀ BACK ▶ NEXT




Once the search criteria are set click “Search”. Clicking “Search” with no search parameter set will list all the existing studies. This is not recommended and it may take a very long time.

Search also can be started by pressing "Enter" in any text box in the Advanced Search area.

On screen opening query will be sent to the default Storage server (one currently selected in the settings screen) but you can switch to another server by selecting it from the list located under search panel

Double click on the row from the list of results or select the row and click “Next” –the matching DICOM files will be stored in the destination folder and then displayed in the [DICOM viewer](#).

Right click on the row opens menu allowing to copy/print patient and study info, add a new series to an existing study or execute some custom action using selected data ("Query action" in the below image):

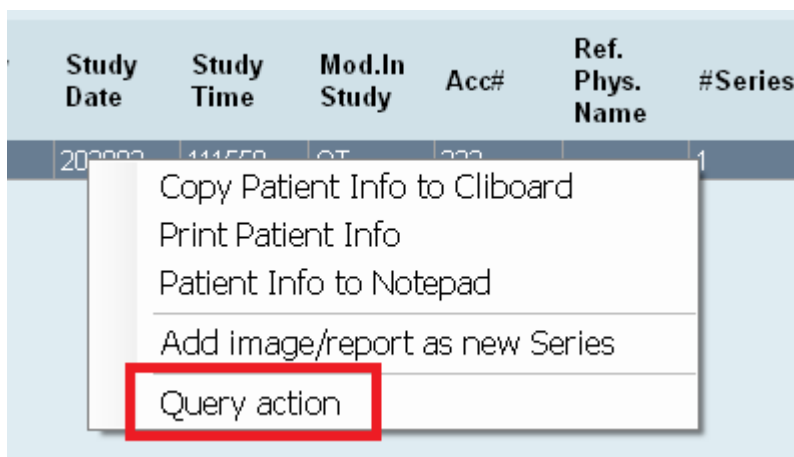

[How to configure Customs Actions](#).

5.6. Export - Burn CD/DVD

MODALIZER+ can create portable medical records with specific studies and reports, and an embedded DICOM Viewer.

Select “Export” from the main screen.

In order to prepare a Standard DICOM Media, MODALIZER+ prepares the media files using standard filenames in Patient-Study-Series-Image hierarchy and creates a DICOMDIR file.



MODALIZER+ | Create DICOMDIR

CREATE DICOMDIR **MODALIZER+**

1 Source Folder [Browse](#) [Scan](#)

PATIENT NAME	PATIENT ID	NUM. of STUDIES	NUM. of SERIES	NUM. of IMAGES
--------------	------------	-----------------	----------------	----------------

2

☒ Rename and arrange DICOM files and create DICOMDIR in place

☐ Copy, arrange and rename DICOM files to a new folder

☐ Just Create DICOMDIR (not recommended)

☐ Include DICOM Viewer to DICOMDIR ☐ Anonymize

Destination Folder [Browse](#)

[SETTINGS](#) | [USER MANUAL](#) X CANCEL ◀ BACK ▶ NEXT

The “Export” screen consists of two areas:

- Part #1:
 - Source Folder - click “Browse” to select the folder with files to burn
 - Study Details Table - click “Scan” to verify the study’s details (if no valid DICOM files found no details will be presented)
- Part #2:

Select the appropriate option from the list:

 - Rename and arrange DICOM files and create DICOMDIR in place - the original DICOM files will be renamed according to the standard and arranged hierarchically and DICOMDIR file will be created in the root folder.
 - Copy, arrange and rename DICOM files to a new folder - the DICOM files will be copied and arranged hierarchically and DICOMDIR will be created in the folder that you define.
 - Just create DICOMDIR (Not recommended) - this option only create DICOMDIR file in the same folder with DICOM files. If the filenames are not according to the standard, they will not be renamed. This option may not comply with all the standard requirements.



- Destination Folder - define the destination folder for the option "Copy, arrange and rename DICOMDIR in folder"

Notes:

- In order to include the Viewer of MODALIZER+ to the created DICOMDIR check the option "Include DICOM Viewer to DICOMDIR".
- In order to anonymize/de-identify DICOM files in the destination folder check the option "Anonymize". This option is available only if "Copy, arrange and rename DICOM files to a new folder" was selected. Also you can select an additional option to remove all private tags (DICOM attributes that are not defined in standard, but are custom data specific for your organization)

Click "Next". Select the drive for the media to be burn. Click "Burn to disc" option.

6. Reporting

MODALIZER+ features two options for creating reports:

1. DICOM Structured Reporting (SR) - The purpose of the DICOM SR specifications is to improve the documentation of diagnostic images by defining semantic reports that can both readable for software and also can be rendered for display. While this method is recommended by the DICOM standard committees, there's no option to control how the report will be displayed by the PACS. If preserving the looks of the report (such as font, colors, logo and other graphic features) is important to you, consider using DICOM Encapsulated PDF Report.
2. Formatted Report Templates – Create PDF reports using the standard DICOM Encapsulated PDF class definition. This option enables controlling the graphic design of the report. MODALIZER+ features a unique templates mechanism to automatically fill the case info into existing template documents.

6.2. Formatted Report Templates

Formatted Report Templates automates the process of filling the report with case attributes such as patient identification (e.g. Name, ID, Birth Date and Sex), study information and other attributes.

A report template is saved as RTF Document with placeholders for values that are automatically filled while following the new patient wizard. You can create your own templates and select from multiple templates depending on the performed procedure.

The special '\$' surrounded placeholders are automatically replaced by the actual attributes values for every new report. The following attributes can be used:



Patient Name	\$PatientName\$
Patient ID	\$PatientID\$
Patient Sex	\$PatientSex\$
Patient Birth Date	\$PatientBirthdate\$
Accession Number	\$AccessionNumber\$
Study Date	\$StudyDate\$
Study Time	\$StudyTime\$
Modality	\$Modality\$
Requested Procedure Description	\$RequestedProcedureDescription\$
Scheduled Procedure Step Description	\$ScheduledProcedureStepDescription\$
Station Name	\$StationName\$
Referring Physicians Name	\$ReferringPhysiciansName\$

Read more about [how to configure the report templates](#).

6.3. DICOM Structured Reports (DICOM SR)

Create a DICOM Structured Report by typing text in the report text panel on "Acquisition" screen and selecting the "DICOM SR" option in the "Create report as" section on "Convert to DICOM" screen. DICOM file containing SR will be added to a destination folder automatically as a separate series. You can load the report to the Viewer where it will be displayed.



7. The Local Archive

The Local Archive is a built-in SQLite database and hierarchically structured storage place (Root folder/Study folder/Series folder/DICOM files). All converted/retrieved from PACS DICOM files are stored in this storage place if "Use local archive" option is marked in Settings screen. You are able to search, view, export, delete stored files and add new DICOM files to an existing study using "Local Archive" screen.

See in "[Settings](#)" how to configure the Local Archive.

Select "Local Archive" from the main screen:

PATIENT NAME	PATIENT ID	SEX	BIRTH DATE	ACCESSI NUMBER	STUDY DATE	STUDY DESCRIP	No OF SERIES	No OF IMAGES	STATUS	INSTITUT NAME	BODY PART EXAMINE
aaa*aaa...	111			222	20200227	DICOMI...	1	3	New		
sdfdds*	3543	M	20200127	34543	20200127	DICOMI...	5	6	New		

Default sorting of the result grid is by study date descending.

Additional search fields are available on opening expander:



MODALIZER+ | Local Archive

LOCAL ARCHIVE
MODALIZER+

ADVANCED SEARCH
[IMPORT FILES](#)
[SEARCH](#)

Patient name: Patient ID: Exact study date: ☐
Accession #: From study date: ☐ To study date: ☐
Institution name: Modality:
Study description: Study part: [CLEAR](#) [SEARCH](#)

PATIENT NAME	PATIENT ID	SEX	BIRTH DATE	ACCESSI NUMBER	STUDY DATE	STUDY DESCRIP	No OF SERIES	No OF IMAGES	STATUS	INSTITUT NAME	BODY PART EXAMINE
aaa*aaa...	111			222	20200227	DICOMI...	1	3	New		
sdfdds^...	3543	M	20200127	34543	20200127	DICOMI...	5	6	New		


[SETTINGS](#) | [USER MANUAL](#)

X CANCEL
BACK
NEXT


Once the search criteria are set click "Search". Double click on the row from the list of results or clicking the "Next" button will lead you to Viewer screen displaying images of the selected study.

You can import DICOM files from the folder by your selection. To do it click "Import files" and select required folder. This folder will be scanned, valid files will be copied to archive folder and found studies will be entered into DB.

Right click on the row opens menu allowing to export/send to PACS/delete selected study or add a new series to it:

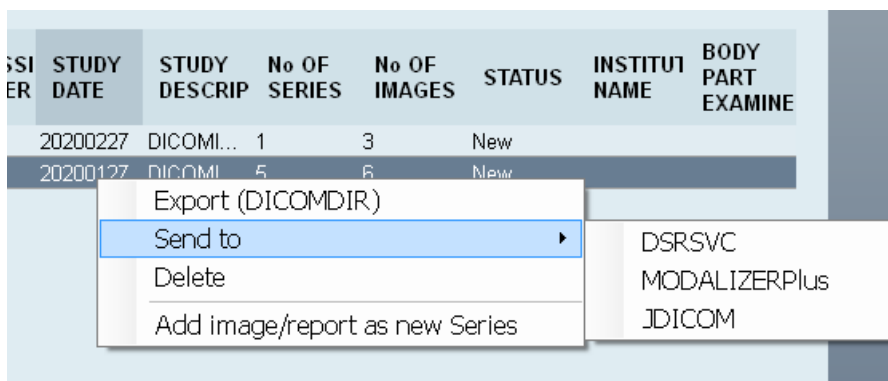

Click on "Export" opens next screen:

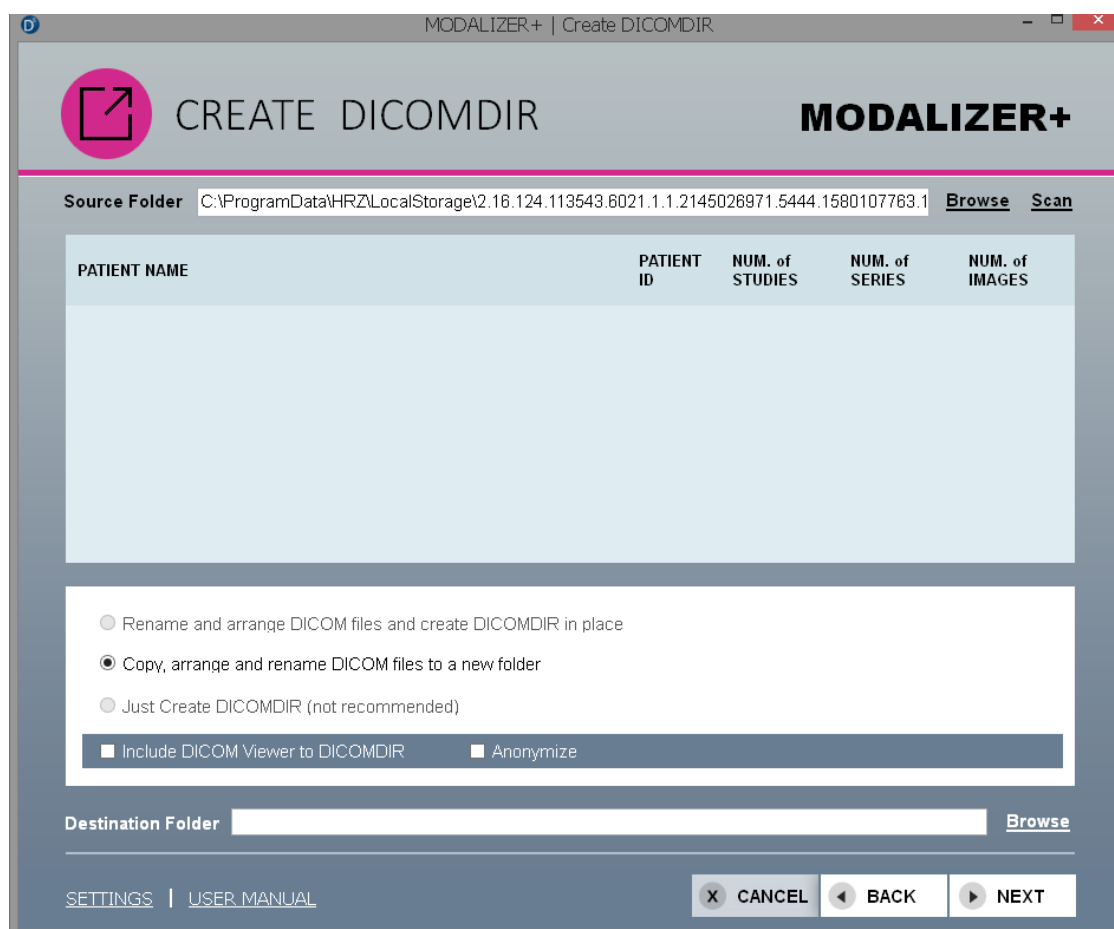



Here you can store images as DICOMDIR on external media (as DVD or Flash drive) or in some folder on your computer (about building DICOMDIRs see [Creating Standard DICOM CD/DVD Exports](#))



8. MODALIZER+ Settings

You can open the “Settings” screen by clicking the “Settings” link in the main menu or by clicking the “Settings” button in the bottom left corner of any screen. Here you can set the Listener, Storage and Worklist servers, configure Local Archive, Formatted report templates and Custom Actions, change the conversion process configuration and define how to display ECG files in the Viewer

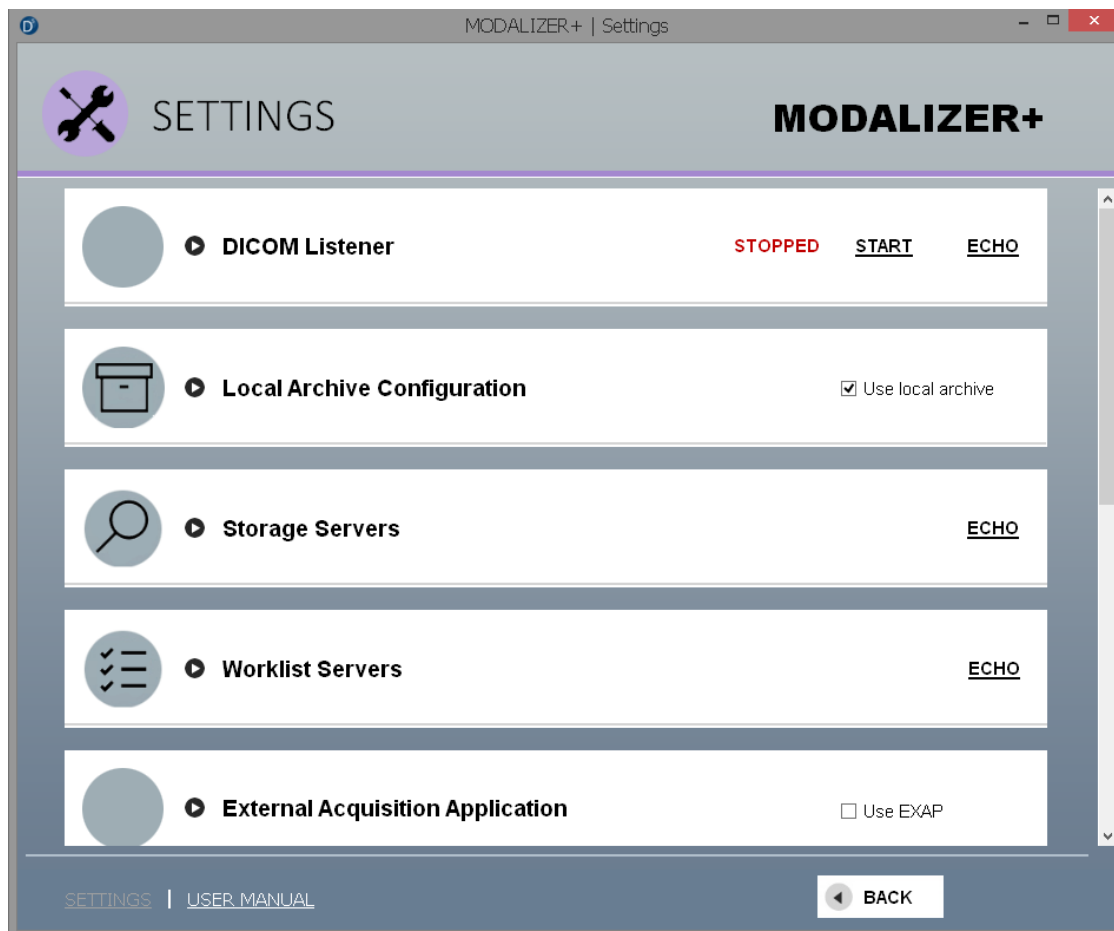

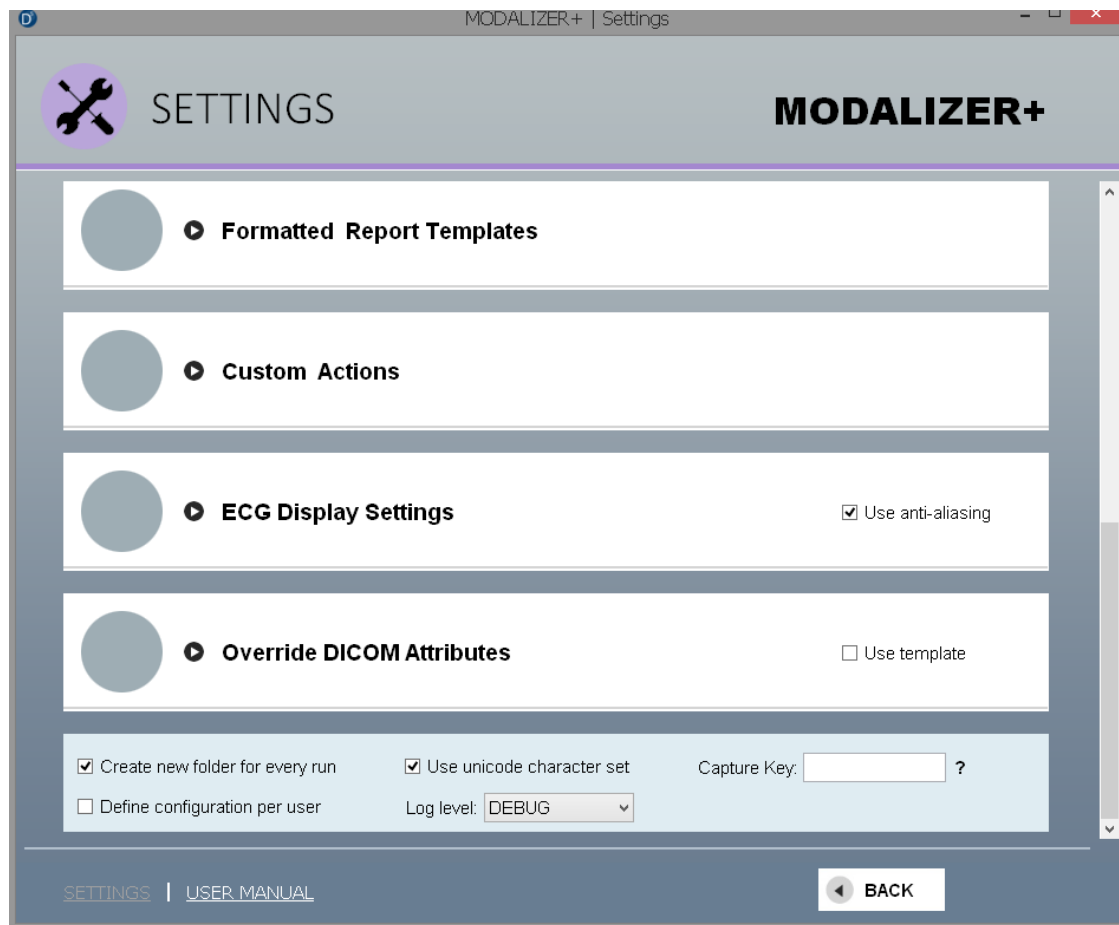


The DICOM nodes (workstations, PACS systems) can communicate if they know each other. That means, each system must know the AE Title, the IP address or hostname and the IP port of the other system. After setting these parameters you will be able to use Storage, Modality Worklist and Query/Retrieve.




8.2. Secure DICOM Networking using TLS (Transport Layer Security)

Certificates from the Windows store can be used to secure the DICOM connections to the PACS. Both the Local Machine and the Current User certificate stores can be used (see Microsoft Management Console).

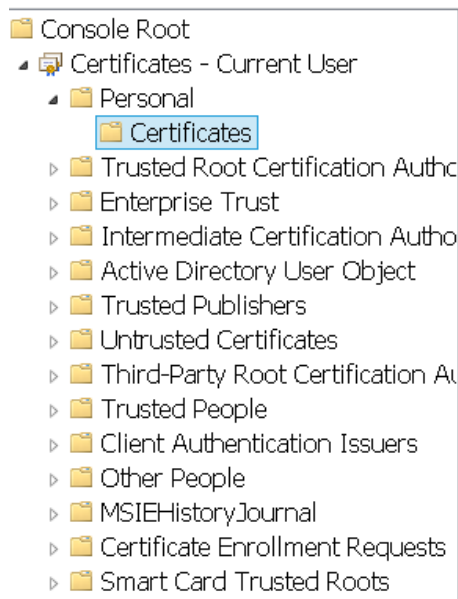

See more detailed explanations about using certificates in Listener configuration and Remote Servers configuration sections.

8.3. DICOM Listener configuration

**DICOM Listener**STOPPEDSTARTECHO

☐ Start listener when application starts

☐ Keep running when listener is on

AE title: Port:

Storage path: BROWSE

☐ Use secure network

Windows Certificates store

MODALIZER+ Certificate: BROWSE CLEAR

Verification method : ☐ Request for Client Certificate (Mutual Authentication)

Approved clients: ADD CLEAR



MODALIZER+ can receive DICOM files sent from other applications if its built-in DICOM Listener is started. Current listener status is displayed in the right upper corner of the Listener tab.

First set your listener AE Title and port. You can always start/stop listener by clicking "Start"/"Stop" button next to status label.


To change folder where listener stores received files - click "Browse" button.

When "Use local archive" on Local Archive configuration tab is selected:


- a. Local Archive folder will be used as listener Storage path and "Browse" button will be disabled.
- b. Info about all DICOM files received by listener will be inserted to DB automatically

You can decide to start listener each time when MODALIZER+ starts by marking "Start listener when application starts" checkbox.

If listener is running there is an indication on the main application screen:

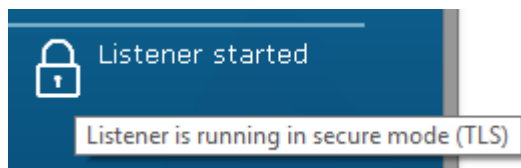

In case "Use secure network" is not selected indication will be like:

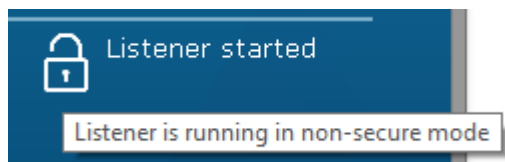

If you want to minimize MODALIZER+ to the tray on closing application by "X" (so that the listener keeps running) - mark "Keep running when listener is on" checkbox. To restore MODALIZER+ to view - right click on tray icon and select "Open". To exit MODALIZER+ which is collapsed to tray - right click on tray icon and select "Exit"

NOTE: If one MODALIZER+ instance is already running, all other instances you'll try to start will be opened in "Viewer only" mode. In such case check for another MODALIZER+ instance collapsed to the system tray.

Checkbox "Use secure network" - if selected enable DICOM TLS Network Security Layer

"Windows Certificate store" area - select required store (Local Machine or Current User)



"MODALIZER+ Certificate" area - click "Browse" to select certificate that identifies MODALIZER+ from Windows store:



Select certificate

Please check that certificate has private key



Issuer: Go Daddy Root Certificate
Authority - G2
Valid From: 03/05/2011 to 03/05/2031

[Click here to view certificate
properties](#)



Go Daddy Root Certificate
Authority - G2
Issuer: Go Daddy Class 2 Certification
Authority
Valid From: 01/01/2014 to 30/05/2031



MySslClientCertificate
Issuer: MySslClientCertificate
Valid From: 01/01/2015 to 01/01/2025



HRZ Software Services LTD
Issuer: Go Daddy Secure Certificate
Authority - G2
Valid From: 23/11/2016 to 21/11/2017



HL7KitCertificate
Issuer: HL7KitCertificate
Valid From: 26/07/2018 to 26/07/2019



NVIDIA GameStream Server
Issuer: NVIDIA GameStream Server
Valid From: 08/03/2019 to 08/03/2039




IIS Express Development
Certificate
Issuer: localhost
Valid From: 19/08/2018 to 19/08/2023

OK

Cancel



If user selects a certificate that doesn't have a private key, an error message will be shown and certificate will not be selected:

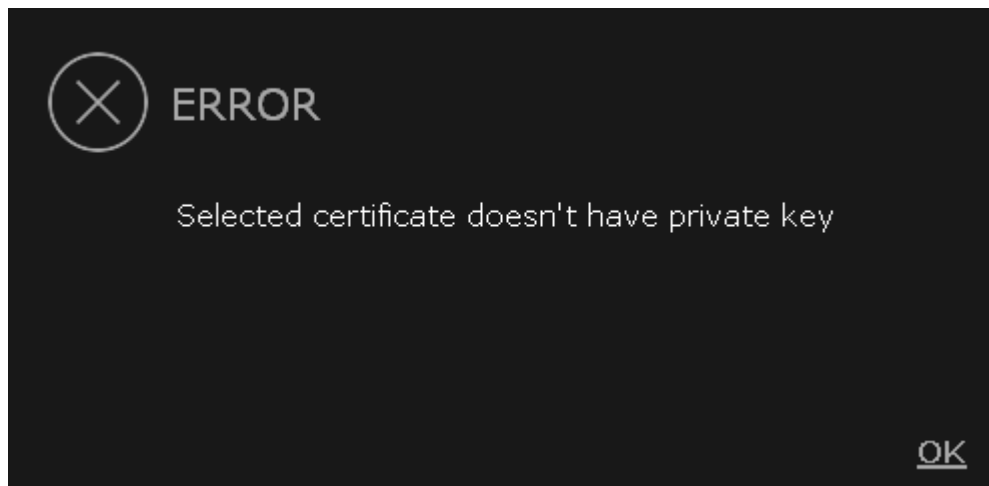

Click "Clear" to remove selected certificate from settings.

Checkbox "Certificate Verification" – if checked listener will ask clients to provide a certificate


Checkbox "Request for Client Certificate (Mutual Authentication)" – when disabled the clients are not asked to identify ???

"Approved clients" textbox - list of all certificates belonging to the listener clients. User must get clients certificates as files and import them into Windows Store using Microsoft Management Console.

Click "Add" to select certificate from the list, click "Clear" to remove ALL client certificates.

8.4. Local Archive configuration

All converted/retrieved DICOM files can be stored in hierarchically structured storage place (Root folder/Study folder/Series folder/DICOM files); info about these files is stored in built-in SQLite data base. To use this option, mark "Use local archive" checkbox on the "Local Archive Configuration" tab.

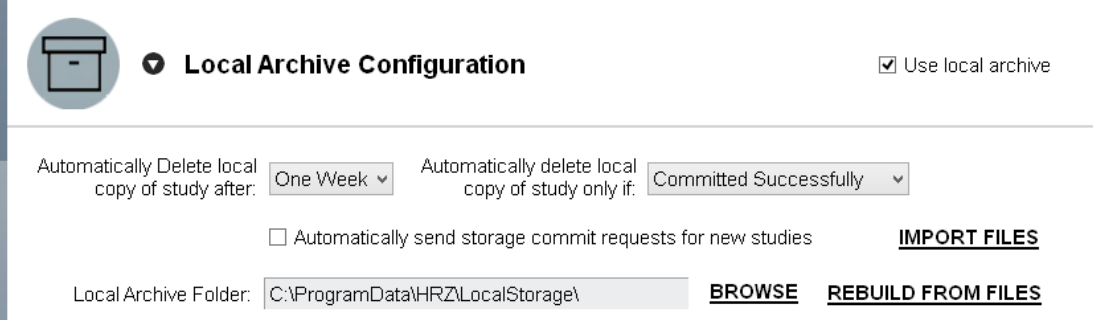

Local Archive Configuration ☒ Use local archive

Automatically Delete local copy of study after: Automatically delete local copy of study only if:

☐ Automatically send storage commit requests for new studies **IMPORT FILES**

Local Archive Folder: **BROWSE** **REBUILD FROM FILES**

To change the root folder where archived studies are stored – click the "Browse" button.

Set required clearing mode by selecting options from "Automatically delete local copy of study after" and "Automatically delete local copy of study only if" lists.

You may need to re-fill DB by info about DICOM files stored in root folder, for example if you want to switch to another storage folder. You can do it by selecting required path and clicking "Rebuild from files" button. Current archive folder will be scanned and found studies inserted into DB.


This operation is executed in separate task with displaying its progress while running. You can stop this operation by clicking "Cancel" button.

Log file RebuildFromFiles.log will be created containing follow data:

- The name of every folder that is scanned
- The name of every file that is opened (full path)
- Whenever new study is added with Study Instance UID.

You can also import DICOM files from the folder by your selection. To do it click "Import files" and select required folder. This folder will be scanned, valid files will be copied to archive folder and found studies will be entered into DB.

8.5. Storage Servers configuration

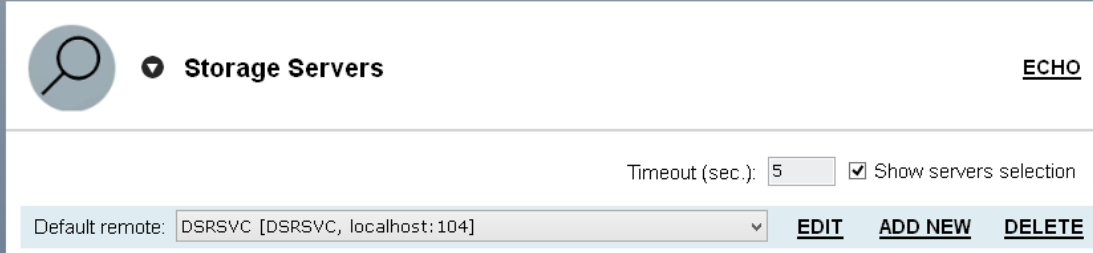

Storage Servers **ECHO**

Timeout (sec.): ☒ Show servers selection

Default remote: **EDIT** **ADD NEW** **DELETE**

Note: You should configure at least one server.

- First set your Local Application Entity Title:



- Local AE - The DICOM AE Title of this installation of MODALIZER+. This must match to the MODALIZER+ AE Title configured in the PACS.
 - Local port - define the port number that MODALIZER+ listens on for incoming connections (The default port is 5108)
 - Timeout - the purpose of a server timeout is to prevent from endlessly waiting for a server to respond. The recommendation is to keep the default, if there are known connection problems increase the value.
- The next step is to define a new server. Click “Add new ”:

DSR SVC

Remote AE: Retrieve method:

Remote host: Remote port:

Description:

Secure network ☐ Windows Certificates store:

Local AE Certificate Subject Name: [Browse](#) [Clear](#)

Verification method:

Remote AE Certificates: [Add](#) [Clear](#)

[Echo](#) [Cancel](#) [Save](#)

Set the data for your Storage Server. Click the “Echo” button to verify that the settings are correct. If red X icon is displayed, verify that the settings are correct and the server is running. Click “Save” to apply the settings for a new Storage Server or “Cancel” to exit the settings. Check the log file lastEcho.log in MODALIZER+ installation folder (C:\MODALIZERPLUS).

"Retrieve method" combo box allows selection between using C-MOVE and C-GET. The user can select which of the commands to use for retrieving the instances.

"Windows Certificate store" area - select required store (Local Machine or Current User)

Local AE Certificate (optional - user don't have to select certificate. Not all servers require it) - click "Browse" to select local certificate from Windows store. Click "Clear" to remove selected local certificate.



This certificate verifies MODALIZER+ identity. The remote AE may request for this (mutual authentication)

Remote AE Certificate (optional - user don't have to select certificate. If not defined MODALIZER+ will not verify the server certificate explicitly) - click "Browse" to select remote certificate from Windows store. Click "Clear" to remove selected remote certificate.

Checkbox "Verify Certificate" (enabled only when Remote AE Certificate is blank) . When checked RZDCX will look for the remote certificate in the local user cert store

Important: To complete this step you must also configure your Storage Server (PACS) with Your MODALIZER+ AE Title (the value you set for "Local AE"), the hostname (or IP address) of your computer and the IP port (the value you set for "Local port").

Note 1: Ask your System/PACS Administrator for the Storage Server parameters.

Note 2: MODALIZER+ is compatible with most DICOM PACS providers. Please advise your PACS software help file about AE configuration of your PACS server or ask your System Administrator.

8.6. Worklist Servers configuration

The Worklist Server must be configured in order to use Modality Worklist query.

The screenshot shows the 'Worklist Servers' configuration panel. At the top left is a circular icon with three checkmarks. The title 'Worklist Servers' is in the center, and 'ECHO' is at the top right. The panel contains the following fields and controls:

- Local AE:** A text input field containing 'ModalitySCU'.
- Timeout (sec.):** A numeric input field containing '5'.
- ☒ **Show servers selection**
- Default worklist:** A dropdown menu showing 'DSRSVC [DSRSVC, localhost:104]'.
- Buttons:** 'EDIT', 'ADD NEW', and 'DELETE' are located to the right of the default worklist dropdown.
- Worklist Query Filter:** A section with three checkboxes: ☐ For today, ☐ For this AE, and ☒ Two step verification.
- Modality:** A dropdown menu.

Configure the parameters for your Worklist Server. Click the "Echo" button to verify that the settings are correct. If red X icon is presented verify that the settings are correct and the server is running. Click "Save" to apply the settings for a new Storage Server or "Cancel" to exit the settings.

Timeout - The recommendation is to keep the default, if there is known connection problem increase the value.

Two more options in the Worklist Server panel refer to Worklist Query filter. You can define that the search results will present only the studies that scheduled for today and/or for a specific Scheduled AE Title. To do this mark the appropriate check-boxes in the "Worklist Server" panel.



"Two step verification" checkbox: if this option is selected (default is checked) – the user will be asked to review and confirm the data received from the Modality Worklist before starting the procedure.

See "Storage servers configuration " about Remote server and security settings.

Checkbox "Automatic MPPS" - select if you want MPPS to be sent with the completed study.

Note: Don't check this option if the Worklist Server you work with doesn't support MPPS.

"Storage server" list allows to select one the remote servers defined in MODALIZER+ as default destination to send study created from the Modality Worklist.

Note: Ask your System Administrator for the Worklist Server parameters.



8.7. External Acquisition Application configuration

User has an option to use some external application to acquire images for converting to DICOM. For example - some application receiving images from medical device as CT etc. This application must receive as input parameter path to some "exchange data" file containing patient data (name and ID) and save acquired file in the parent folder of this file.

To use this option, the following parameters must be configured in the settings screen:

1. **Path to executable:** full path to EXE file starting external application (by default it is built-in example working exactly as Acquisition screen). To select EXE - click "Browse" button in the same line. To return to built-in example - click "Reset to built-in" button
2. **Shared folder:** full path to a folder in which exchange file (XML, txt, json etc.) will be stored. To select folder - click "Browse" button in the same line.

In order to use EXAP - select **"Use EXAP"**

When "Use EXAP" is selected - external application will be started when user clicks "Next" button on "New patient"/ "Modality Worklist" screen or on adding new series to existing study from "Local Archive"/"Query Retrieve" screen.

MODALIZER+ will fill the exchange file with case attributes such as patient identification (e.g. Name, ID, Birth Date and Sex), study information and other attributes.

Template file (located in MODALIZER+ installation folder and named **PatientDataTemplate.xml**) can be of any text format - XML, txt, json, even RTF. By default it's XML containing ALL available fields:

```
<?xml version="1.0" encoding="utf-8" ?>
<PatientData>
  <PatientName>
```




```
        $PatientName$
    </PatientName>
    <PatientId>
        $PatientID$
    </PatientId>
    <PatientSex>
        $PatientSex$
    </PatientSex>
    <PatientBirthdate>
        $PatientBirthdate$
    </PatientBirthdate>
    <AccessionNumber>
        $AccessionNumber$
    </AccessionNumber>
    <StudyInstanceUID>
        $StudyInstanceUID$
    </StudyInstanceUID>
    <StudyId>
        $StudyId$
    </StudyId>
    <StudyDate>
        $StudyDate$
    </StudyDate>
    <StudyTime>
        $StudyTime$
    </StudyTime>
    <Modality>
        $Modality$
    </Modality>
    <RequestedProcedureDescription>
        $RequestedProcedureDescription$
    </RequestedProcedureDescription>
    <ScheduledProcedureStepDescription>
        $ScheduledProcedureStepDescription$
    </ScheduledProcedureStepDescription>
    <StationName>
        $StationName$
    </StationName>
    <ReferringPhysiciansName>
        $ReferringPhysiciansName$
    </ReferringPhysiciansName>
</PatientData>
```

Output file is saved as PatientData.xml in the shared folder so your EXAP application is able to load required data from it.

The special '\$' surrounded placeholders are automatically replaced by the actual attributes values for every new exchange file.




MODALIZER+ is installed with built-in EXAP application as example:

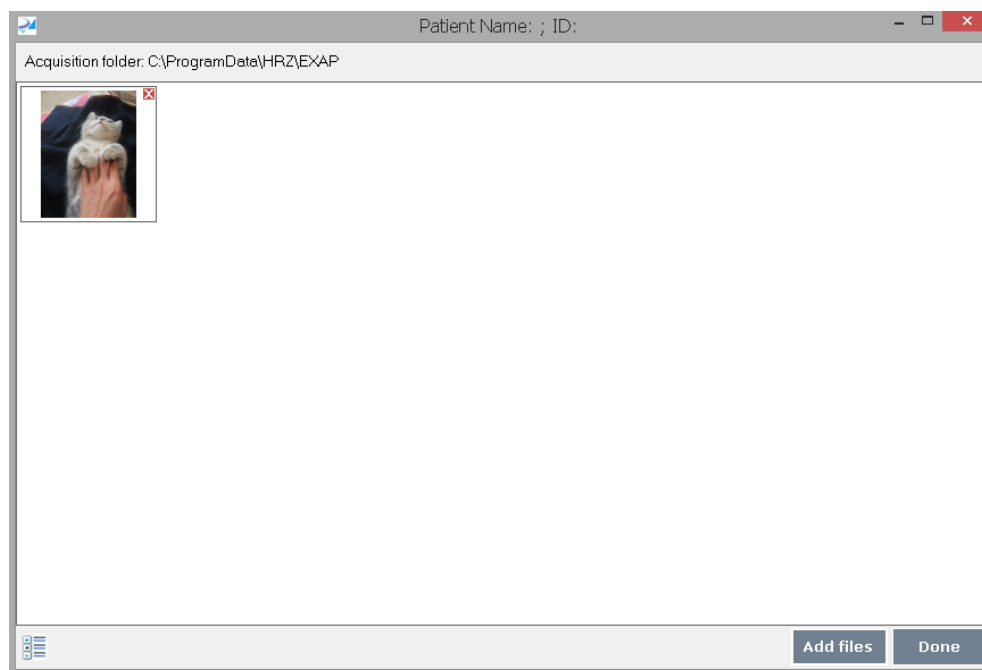

After user added files and clicked "Done" (or executed custom actions in external application and closed it) - "Acquisition" screen will be opened with acquired files added to the list

8.8. Formatted Report Template configuration

About formatted reports structure see [Reporting](#) section.

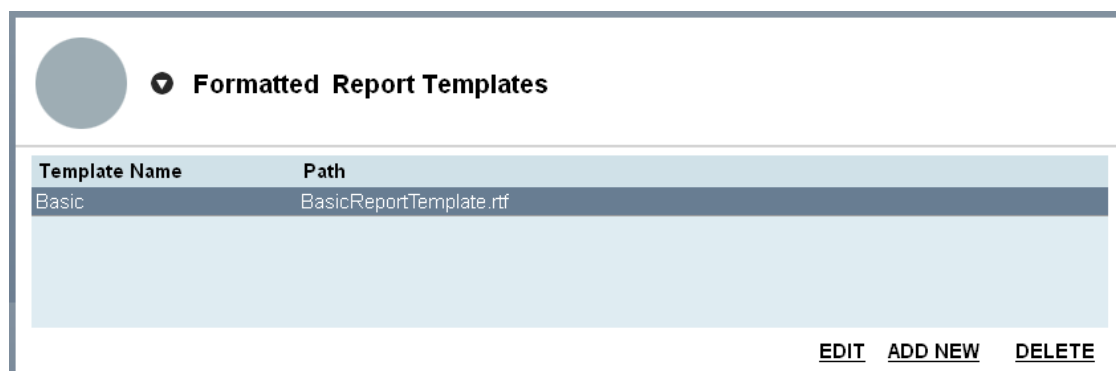

Select required template in the list and click "Edit" to edit the template properties:



Edit formatted report

Template Name

Basic

Edit template

Path

BasicReportTemplate.rtf

Browse

Cancel

Save

You can change templates name which is displayed in the list of templates on "Images" screen, select another RTF file or open RTF file itself to edit its content by clicking "Edit template" button (you can edit the header/footer of the template, edit text and add Logo).

If you want to create a new template - click "Add new" and select path to your custom RTF file.

To delete existing template - select it in the list and click "Delete"

NOTE: At least one template must exist so you cannot delete last one.

8.9. Custom Actions configurations

"Custom Action" is a some operation you can execute using data from one MWL entry (see [Modality Worklist Query](#)) or Query entry (see [Query/Retrieve - Searching the PACS](#))

Custom Actions

Start from	Title	Command	Replace Params
Modality Worklist	test	C:\Temp\test.rtf	<input checked="" type="checkbox"/>
Query Retrieve	Query action	Some.exe	<input type="checkbox"/>

EDIT

ADD NEW

DELETE

To create new custom action click "Add new" button:



New custom action

Start from: Modality Worklist

Title:

Command: Browse

Replace parameters: ☐

Test Cancel Save

Select a screen where you want to see new action (Modality Worklist or Query Retrieve), give action a title which will appear in the list and define some command you want to execute - path to some file (as .TXT, .RTF, .EXE or .BAT) .

Mark "Replace parameters" checkbox to make application replace pre-defined parameters inside command file by data from MWL/Query (as in [formatted report](#))

When you select custom action from the row on MWL/QUERY screen - defined file will be opened (with replaced parameters if needed) as separate system process.

To edit existing custom action - select it in the list and click "Edit" button.

To delete existing custom action - select it in the list and click "Delete" button.

You can test your action by clicking "Test" button (parameters will be replaced by some random data).

Types of the custom action:

1. Start EXE without parameters.
2. Open document template, TXT or RTF for example, containing placeholders (\$PatientID\$ etc.) to replace (like formatted reports). Place holders will be replaced, files stored in [MyDocuments]\MODALIZERPLUS\ACTIONS folder and opened as separate process (Notepad, Word etc.)
3. Start EXE with parameters. To pass parameters to EXE you need to do follow:
 - a. Create batch file containing path to your EXE and parameters, for example MyCustomAction.bat file which content is
"C:\MyFolder\EXE.exe \$PatientID\$ \$PatientName\$ "



- b. Select MyCustomAction.bat as you custom action.
- c. Select "Replace parameters" check box.

Available parameters are:

\$PatientName\$
 \$PatientID\$
 \$PatientSex\$
 \$PatientBirthdate\$
 \$StudyDate\$
 \$AccessionNumber\$
 \$StudyTime\$
 \$Modality\$
 \$RequestedProcedureDescription\$
 \$ScheduledProcedureStepDescription\$
 \$StationName\$
 \$ReferringPhysiciansName\$

8.10. DICOM templates - Override DICOM Attributes

DICOM attributes are stored in the files that you can edit or replace. In order to use the attributes as they're defined in the template mark "V" in the check-box "Use Template".

Application allows to define not only one template common to all converted DICOM files, but also specific templates for each type of such files.

There is combo box "Type" in "Override" section:

Override DICOM Attributes ☐ Use template

Type: **Common** Path to template file: D:\Temp\template2.dcm **BROWSE** **NEW**

Fill header tags to put in the created objects (overrides anything else) ☒

Search: Name: N#: **ADD**

Tag name	Tag name	Value	Length	VR
X (0008,0090)	ReferringPhysicianName		0	PN

"Common" template (if defined) will be inserted into each converted DICOM file.

There are also four other types: Image, PDF, Video and Structure Report templates which will be inserted only to relevant files.



Any of the files can be created/selected separately.

Important! The override attributes are applied after all other conversion steps were made. Make sure not to override any image attributes (group 0028).

To create your own DICOM attributes template click "New", in the opened window select the file location and give it a name. Click "Save". The created file will be automatically loaded in MODALIZER+ and you can edit the attributes. You can find the attribute by its name - start typing to get a drop-list of the appropriate attributes or search by the attribute's tag enumeration. Click "Add" to present the value in the table. Enter the new value in the attribute's row in the "Value" column. Clicking "X" in the left column will remove the attribute from the template.

If you want to use another DICOM attributes template click "Browse" and select.

8.11. ECG Display Settings

See [Displaying ECG in Viewer](#).

8.12. Misc configuration

At the bottom of the configuration screen there are few additional options:

The screenshot shows a light blue rectangular box containing several configuration options. On the left, there are two checkboxes: 'Create new folder for every run' (checked) and 'Define configuration per user' (unchecked). In the middle, there is a checked checkbox for 'Use unicode character set' and a 'Log level' dropdown menu currently set to 'DEBUG'. On the right, there is a 'Capture Key' field with a text input box and a question mark icon.

8.12.1. File System Directory Organizations

Create new folder for every run - in this way each study will be stored in separated folder (Recommended).

When Local Archive is disabled the converted images destination folder can be manually set (see [New Patient](#)).

When "Create new folder" is enabled, every study is stored in a newly created directory.

8.12.2. Support of the Unicode character set

When "Use unicode caharcter set" is checked, values of "String" tags (Value Representation SH, LO, ST, LT, UT, PN) will be inserted encoded as Unicode.

8.12.3. Per-User Configuration

When per-user configuration is checked, every user (from the windows operating system) has its own configuration file.



8.12.4. Capture Key

Define key combination to capture image from the currently selected TWAIN/WIA device when in the capture screen

1. click inside the "capture key" text box
2. Hold the keys combination to use for image capture.


Valid keys:

- Combinations of control/alt/shift keys and characters (Ctrl-A, Alt-Z, Ctrl-Shift-F etc.)
- The function keys (F1, F2, ...)

Enter/Return and Space keys are not recommended as they may interfere with standard UI functionality.

To disable the capture key, click in the text box and then press the delete key.

8.12.5. DICOM Log level for operations as "Send ECHO", "Get Query" etc.

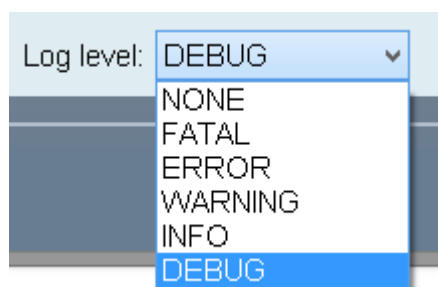

Default value is "INFO"



9. Completing tasks with MODALIZER+

9.2. Viewing DICOM Images

MODALIZER+ is a powerful DICOM Workstation that lets you display DICOM Files from your local computer, from CD/DVD/USB and from any PACS.

There are a few ways to present the files - you can Drag-and-drop the items or to click “Open Files” to browse for a folder and select the files to view. In order to present all folder’s content use “Open Folder” button.

9.3. Using CD/DVD DICOM Viewer

DICOMZIER automatically adds a DICOM CD Viewer to every burned CD/DVD so patients and physicians can view their studies and reports anywhere. Double click the DICOM Viewer application in the CD/DVD root folder to view the CD/DVD content.

9.4. Viewing PDF file in DICOM format

To extract a PDF from a DICOM Encapsulated PDF file, click PDF icon in the Viewer – the file will be converted to PDF and displayed using your system default PDF viewer.

9.5. Attaching scanned documents to the patient folder

MODALIZER+ will automatically identify compatible camera or other imaging device connected to your computer. If there are more than one device connected choose the one you’d like to use through the drop-list in the upper left corner of the Image/Report panel.

Capture an image by clicking on the red button. The icon of the captured image will be presented in the panel below the Image/Report panel.

9.6. Sending the same study to multiple destinations

Once an operation is completed you can send a copy of your study to others DICOM applications by using the “Send to” option in the operation completed screen. Select the destination from the drop-list next to the “Send to” button. If the destination DICOM application is not in the list, enter settings and add new [Storage Server](#).

9.7. MPPS (Modality Performed Procedure Step)

Modality Performed Procedure Step is a complementary service to Modality Worklist.

Once the procedure was started via Modality Worklist Query the modality creates a new MPPS that references the Study.



MPPS has 3 statuses:

- IN PROGRESS – this means that the procedure has been started
- COMPLETED – this means that the procedure is finished.
- DISCONTINUED – if the procedure was stopped in the middle

10. Troubleshooting


10.2. Log Files

MODALIZER+ Log files are stored in the directory: C:\Users\<User>\Documents\MODALIZERPLUS\LOGS.

MODALIZER+ keeps the last log for every DICOM operation:

- LastEchoToStorageServer - the log on Echo to PACS action
- LastEchoToWorklistServer - the log on Echo to Worklist Server action
- LastMove - the log on copying a study to PACS
- LastMPPSCreate - the log on MPPS creation
- LastMPPSSet - the log on setting MMPS
- LastQuery - the log on Query Retrieve operation
- LastSend - the log on the send to PAXS operation
- LastWorklistQuery1 - the log on Worklist Server search operation

When operation fails, message will be displayed with an option to open correspondent Log file:

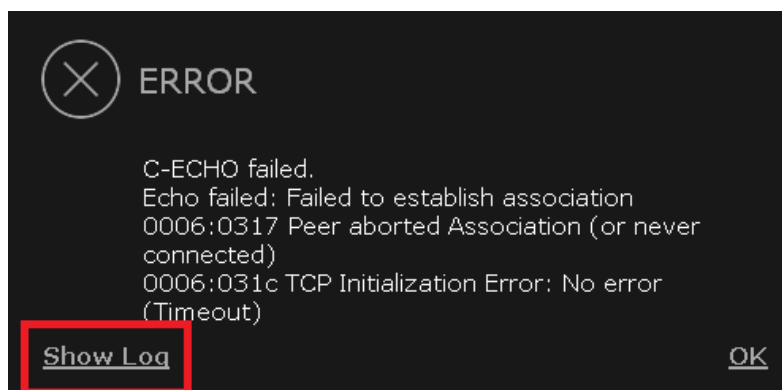



11. Command line parameters

When launched with specified command line parameters MODALIZER+ will start directly in the Q/R screen and send a query according to the parameters. Query parameters appear in the query screen when results are retrieved from PACS and could be editable for additional query.

Also there is command line parameter allowing to get "snapshot" of the current image from the MODALIZER+ viewer.

Command Line options

-q or -Q	Start MODALIZER+ in the query screen and send a Query.
-o or -O	Set the output path for Send as references. This option overrides the EXAP shared folder name.

Query parameters

0 or more query parameters can follow the -Q option. Every parameter should be of the form:

tagName="value"

Double quotes are optional for cases where the value contains whitespace characters (space).

The allowed tags are all the ones that are displayed in the Q/R screen including the advanced search. The tag names should be according to RZDCX's DICOM TAG ENUM.

Option	Tag Name	Tag	Comments and examples
patientName	Patient Name	(0010,0010))	
patientId	Patient ID	(0010,0020))	
PatientBirthDate	Patient Birth Date	(0010,0030))	Exact date in DICOM format (YYYYMMDD) Example: "20170821"
PatientSex	Patient Sex	(0010,0040))	Valid Values: M/F/O or Male/Female/Other (both accepted).
AccessionNumber	Accession Number	(0008,0050))	



StudyDate	Study Date	(0008,0020)	Exact date in DICOM format (YYYYMMDD) including ranges. When value is a date range double quotes must be used to prevent parsing it as command line option. Examples: "20170821" (exact date) "-20170821" (to date). "20170812" (from date). "20170812-20170911" (date range)
ModalitiesInStudy	Modalities in Study	(0008,0061)	

Example: MODALIZERPlus.EXE -q patientId="111" will start the directly to the Q/R string and start a query:

MODALIZER+ | Query Retrieve | DSR SVC

QUERY RETRIEVE **MODALIZER+**

Advanced Search [SEARCH](#)

Patient name: Accession number:

Patient ID: Study date: ☐

Patient birth date: ☐ Study from: ☐ To: ☐

Patient Sex: Modalities in study: [CLEAR](#) [SEARCH](#)

Destination Folder:

Studies list (to retrieve selected study double-click on the row or select row in the grid and click "Next")


Patient Name	Patient ID	Birth Date	Sex	Study ID	Study Date	Study Time	Mod.In Study	Acc#	Ref. Phys. Name	#Series	#Inst	Study Instance UID
aaa^aa...	111			1	202002...	111558...	OT	222		1	3	2.16.12...

[SETTINGS](#) | [USER MANUAL](#)



Save as reference button

When the -O command line parameter is used, the Save as reference button will be displayed instead of the three buttons on the left (open file, open folder and history) :

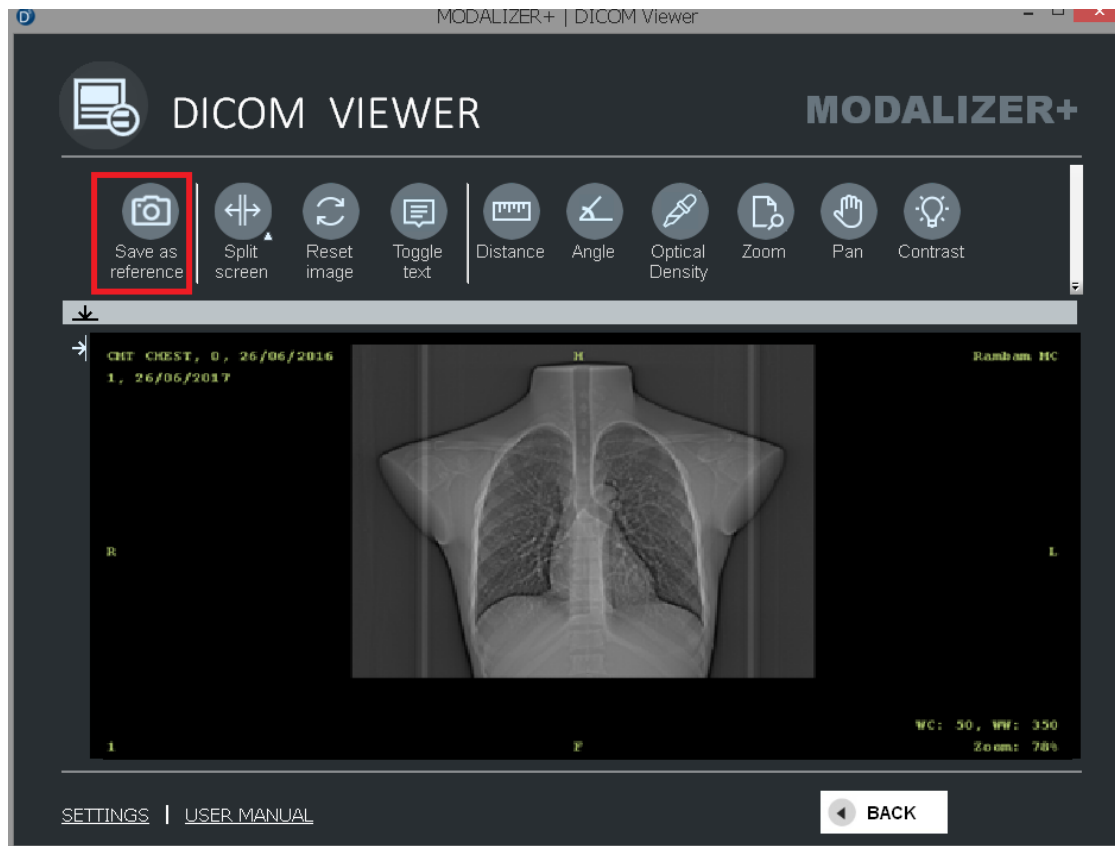

Clicking the "Save as reference" button will save the currently displayed and selected image using the current VOI LUT to the path provided as the value of the option. For example if the MODALIZER+ started with the command: *MODALIZERPlus.EXE -O "c:\taken Send as references"* then the files will be saved in "c:\taken Send as references".

The Save as references will be saved in PNG format in the full resolution of the DICOM image (i.e. according to the Rows and Columns tags (0028,0100) and (0028,0101).

Next to the PNG file, the original DICOM file will be saved:

The Send as reference save files will have the following filename pattern:

<destination-folder>\SOP Instance UID.png
<destination-folder>\SOP Instance UID.dcm



<destination-folder> is the value from the -O command line parameter. If -O is not set, application uses the EXAP shared folder from configuration.

If the provided path is not empty, and there is already a file with that name, the file shall be replaced without asking the user.

Start MODALIZER+ with "-help" or "-h" parameter to open popup windows with the description of command line parameters.

